



National Library
of Canada

Bibliothèque nationale
du Canada

Canadian Theses Service / Services des thèses canadiennes

Ottawa, Canada
K1A 0N4

CANADIAN T H E S E S

THÈSES CANADIENNES

NOTICE

The quality of this microfiche is heavily dependent upon the quality of the original thesis submitted for microfilming. Every effort has been made to ensure the highest quality of reproduction possible.

If pages are missing, contact the university which granted the degree.

Some pages may have indistinct print especially if the original pages were typed with a poor typewriter ribbon or if the university sent us an inferior photocopy.

Previously copyrighted materials (journal articles, published tests, etc.) are not filmed.

Reproduction in full or in part of this film is governed by the Canadian Copyright Act, R.S.C. 1970, c. C-30. Please read the authorization forms which accompany this thesis.

AVIS

La qualité de cette microfiche dépend grandement de la qualité de la thèse soumise au microfilmage. Nous avons tout fait pour assurer une qualité supérieure de reproduction.

S'il manque des pages, veuillez communiquer avec l'université qui a conféré le grade.

La qualité d'impression de certaines pages peut laisser à désirer, surtout si les pages originales ont été dactylographiées à l'aide d'un ruban usé ou si l'université nous a fait parvenir une photocopie de qualité inférieure.

Les documents qui font déjà l'objet d'un droit d'auteur (articles de revue, examens publiés, etc.) ne sont pas microfilmés.

La reproduction, même partielle, de ce microfilm est soumise à la Loi canadienne sur le droit d'auteur, S.R.C. 1970, c. C-30. Veuillez prendre connaissance des formules d'autorisation qui accompagnent cette thèse.

THIS DISSERTATION
HAS BEEN MICROFILMED
EXACTLY AS RECEIVED

LA THÈSE A ÉTÉ
MICROFILMÉE TELLE QUE
NOUS L'AVONS REÇUE

Canada



National Library of Canada

Bibliothèque nationale du Canada

B-315-24801-7

Canadian Theses Division / Division des thèses canadiennes

Ottawa, Canada
K1A 0N4

PERMISSION TO MICROFILM — AUTORISATION DE MICROFILMER

• Please print or type — Ecrire en lettres moulees ou dactylographier

Full Name of Author — Nom complet de l'auteur

Yvette Chan CLAUPEAU

Date of Birth — Date de naissance

DEC 3 1948

Country of Birth — Lieu de naissance

CANADA

Permanent Address — Residence fixe

7621-46 AVE EDMONTON ALTA.

Title of Thesis — Titre de la thèse

The effect of Shortwave Diathermy, Ultrasound and Hot Packs on Human Motor Nerve Conduction Velocity

University — Université

University of ALBERTA

Degree for which thesis was presented — Grade pour lequel cette thèse fut présentée

MSc

Year this degree conferred — Année d'obtention de ce grade

1954

Name of Supervisor — Nom du directeur de thèse

Dr David Magee

Permission is hereby granted to the NATIONAL LIBRARY OF CANADA to microfilm this thesis and to lend or sell copies of the film.

L'autorisation est, par la présente, accordée à la BIBLIOTHÈQUE NATIONALE DU CANADA de microfilmer cette thèse et de prêter ou de vendre des exemplaires du film.

The author reserves other publication rights, and neither the thesis nor extensive extracts from it may be printed or otherwise reproduced without the author's written permission.

L'auteur se réserve les autres droits de publication; ni la thèse ni de longs extraits de celle-ci ne doivent être imprimés ou autrement reproduits sans l'autorisation écrite de l'auteur.

Date

August 01 1954

Signature

Yvette D. Chaupeau

THE UNIVERSITY OF ALBERTA

Effects of Shortwave Diathermy, Ultrasound, and Hot Packs on Ulnar
Motor Nerve Conduction Velocity

by



Yvette D. Claveau

A THESIS

SUBMITTED TO THE FACULTY OF GRADUATE STUDIES AND RESEARCH
IN PARTIAL FULFILLMENT OF THE REQUIREMENTS FOR THE DEGREE
OF Master of Science

Department of Physical Therapy

EDMONTON, ALBERTA

Fall 1984

THE UNIVERSITY OF ALBERTA
RELEASE FORM

NAME OF AUTHOR Yvette D. Claveau
TITLE OF THESIS Effects of Shortwave Diathermy, Ultrasound, and
 Hot Packs on Ulnar Motor Nerve Conduction Velocity
DEGREE FOR WHICH THESIS WAS PRESENTED Master of Science
YEAR THIS DEGREE GRANTED 1984

Permission is hereby granted to THE UNIVERSITY OF ALBERTA LIBRARY to reproduce single copies of this thesis and to lend or sell such copies for private, scholarly or scientific research purposes only.

The author reserves other publication rights, and neither the thesis nor extensive extracts from it may be printed or otherwise reproduced without the author's written permission.

(SIGNED) *Yvette D. Claveau*.....

PERMANENT ADDRESS:

..... 7621 40 Avenue.....
..... Edmonton, Alberta.....
..... Canada T6K 1V5.....

DATED ..August.3..... 1984

THE UNIVERSITY OF ALBERTA
FACULTY OF GRADUATE STUDIES AND RESEARCH

The undersigned certify that they have read, and recommend to the Faculty of Graduate Studies and Research, for acceptance, a thesis entitled Effects of Shortwave Diathermy, Ultrasound and Hot Packs on Ulnar Motor Nerve Conduction Velocity submitted by Yvette D. Claveau in partial fulfilment of the requirements for the degree of Master of Science

Department of Physical Therapy,

David M. Aggar

Supervisor

J. H.

John H. Kramer

John H. Kramer

Date *August 3, 1954*

DEDICATION

This thesis is dedicated to Marion. Thank you for your critique sense of humour and confidence.

ABSTRACT

The effects of a 20 minute treatment of shortwave diathermy, a five minute treatment of ultrasound at an intensity of one watt per square centimeter continuous current, and a 20 minute application of hot pack on the subcutaneous tissue temperature of a 10-12 centimeter segment of the proximal antero-medial aspect of the forearm and the motor nerve conduction velocity of the ulnar nerve was examined in 18 subjects. Each subject was tested three times, using one of the modalities on each test. Only the dominant arm was used. Subcutaneous tissue temperature and motor nerve conduction velocity data were collected four times during the procedure: 1) one minute pre-treatment, 2) zero minute pre-treatment, 3) zero minute post-treatment, and 4) one minute post-treatment. A subcutaneous tissue layer measurement of the triceps and the forearm was taken on each subject. A two by three way analysis of variance with repeated measurements over two factors was used to analyze the data. The results indicated that application of shortwave diathermy and hot packs produced a significant increase in subcutaneous tissue temperature and motor nerve conduction velocity of the ulnar nerve. There was no statistically significant change in subcutaneous tissue temperature or motor nerve conduction velocity with ultrasound. The Pearson Product Correlation Coefficient demonstrated a statistically significant correlation between the change in subcutaneous tissue temperature and the change in motor nerve conduction velocity with hot packs only. No other statistically significant correlation was found between the change in subcutaneous tissue temperature, the change in motor nerve conduction velocity, and the skinfold thickness layer.

ACKNOWLEDGEMENTS

My sincere thanks to: Dr. David Magee, Chairman of my thesis committee and Dr. John Kramer, Dr. Anne Bellamy, and Dr. George Monckton, committee members. I am grateful for the guidance I received and appreciate the time and effort these individuals provided during the process of this thesis.

Further appreciation is extended to Mr. C. Humphrey, Computing Services, University of Alberta, Mary Ann Hickey, my very dedicated typist, Dr. Jim Vargo for his assistance in the data analysis, and all of the subjects who so willingly participated. Without their help this thesis could not have been completed.

Lastly, I would like to thank my family for their care, love, and support.

Table of Contents

Chapter	Page
A. CHAPTER I - THE PROBLEM	1
RESEARCH HYPOTHESES	7
OBJECTIVES	7
OPERATIONAL DEFINITIONS	7
DELIMITATIONS	8
LIMITATIONS	8
REFERENCES - CHAPTER I	10
B. CHAPTER II - REVIEW OF THE LITERATURE	12
SHORTWAVE DIATHERMY	12
ULTRASOUND	13
HOT PACKS	16
NERVE CONDUCTION VELOCITY	17
NEUROPHYSIOLOGICAL MECHANISM OF NERVE CONDUCTION	17
CONCLUSION	20
REFERENCES - CHAPTER II	22
C. CHAPTER III - METHODS AND PROCEDURES	24
EXPERIMENTAL SUBJECTS AND EQUIPMENT	24
CALIBRATION OF EQUIPMENT	29
EXPERIMENTAL PROCEDURE	30
STATISTICAL PROCEDURE	35
RISKS AND PRECAUTIONS	36
REFERENCES - CHAPTER III	37
D. CHAPTER IV - THE RESULTS	38
E. CHAPTER V - DISCUSSION	47
REFERENCES - CHAPTER V	54
F. CHAPTER VI - CONCLUSION	55
G. BIBLIOGRAPHY	57
H. APPENDIX A - FORMS USED IN RESEARCH PROJECT	62
QUESTIONNAIRE FOR SCREENING POTENTIAL SUBJECTS	63

	INFORMED CONSENT FORM FOR EXPERIMENT	65
	INFORMATION TO POTENTIAL SUBJECTS	66
I.	APPENDIX B - CALIBRATION OF EQUIPMENT	68
J.	APPENDIX C - RELIABILITY TESTS AND PROCEDURES	77
K.	APPENDIX D - RAW DATA COLLECTION FORMS	81

LIST OF TABLES

TABLE	DESCRIPTION	PAGE
1	Comparison of the Absorption and the Transmission of Shortwave Diathermy, Ultrasound and Hot Packs in Different Body Tissues.	6
2	Assignment of Treatment Sequences to Subjects	24
3	Obesity Standards	25
4	Percent Error Tests for Measurement of Skinfold Thickness Layer, Measurement of Conduction Velocity, and Placement of Electrode	39
5	Correlation Coefficients for One and Zero Minute Pre-Treatment and Zero and One Minute Post-Treatment on Subcutaneous Tissue Temperature and Motor Nerve Conduction Velocity	39
6	Mean and Standard Deviation of Zero Minute Pre- and Zero Minute Post-Treatment Subcutaneous Tissue Temperatures and Motor Nerve Conduction Velocities For Shortwave Diathermy, Ultrasound, and Hot Packs	40
7	Change in Subcutaneous Tissue Temperature and Motor Nerve Conduction Velocity Following the Application of Shortwave Diathermy, Ultrasound, and Hot Packs	40
8	Analysis of Variance for Subcutaneous Tissue Temperature	41
9	Analysis of Variance for Motor Nerve Conduction Velocity	42

10	Newman-Keuls Test Probability Summary for Subcutaneous Tissue Temperature	44	ii
11	Newman-Keuls Test Probability for Motor Nerve Conduction Velocity	45	
12	Correlation Matrices for Change in Subcutaneous Tissue Temperature, Change in Motor Nerve Conduction Velocity, and Skinfold Thickness for Each Modality	46	
13	Comparison of Mayer's Standard of Minimum Triceps Skinfold Thickness Indicating Obesity and Triceps Skinfold Thickness of Subjects	51	

LIST OF FIGURES OR ILLUSTRATIONS

FIGURE	DESCRIPTION	PAGE
1	Tissue Temperature Change Following the Application of Shortwave Diathermy and Ultrasound	2
2	Temperature Distribution at the Completion of 20 Minutes of Shortwave Diathermy	3
3	Tissue Temperature Change at Skin Surface 3.0 and 4.5 Centimeters During the Application of Ultrasound	4
4	Tissue Temperature Change at Skin Surface 2.0 and 3.9 Centimeters During 20 Minutes of Application of Hot Pack	5
5	Position of Subject During Experimental Procedure	27
6	Equipment and Modalities Used in Experiment	31
7	Electromyograph Timer, Digital Thermometer, Needle Probes, and Gra-lab Timer	32
8	Change in Subcutaneous Tissue Temperature During the Application of Ultrasound	49
9	Russian Ultrachallersdungomessgerat Vmy-3 Unit With Burdick Ultrasound Unit	70
10	Calibration of a Needle Probe with the Digital Thermometer	72

A. CHAPTER I - THE PROBLEM

Motor nerve conduction velocity has been shown to increase as tissue temperature is raised⁹. Heating modalities such as shortwave diathermy, ultrasound, and hot packs are frequently used as part of physical therapy treatments, yet little is known concerning the specific physiological effects of each modality on motor conduction velocity¹⁰. An important factor influencing change of motor nerve conduction velocity is variations in the temperature in the tissue surrounding the nerve¹¹. As each modality has different depths of penetration and different selective tissue heating, it might be postulated that each modality will produce different heating effects in the tissue surrounding the nerve¹¹.

Shortwave diathermy is known to heat predominately tissue of higher fluid content such as muscle and blood vessels^{10 11}. As well, it is not easily transmitted through fatty tissue¹¹.

Ultrasound is easily transmitted through fatty tissue¹². Reflection of ultrasound occurs at bone-soft tissue interface. Therefore, additional heating effects will occur at the bone-soft tissue interface due to the reflection of the ultrasound¹³. In addition to the heating effect, ultrasound has been reported to have a mechanical or vibromassage effect on tissue⁴.

Hot packs are a form of conductive heat and, as such, have only a superficial heating effect¹¹. Lehmann, et al.¹⁴ demonstrated that hot packs produce an increase in tissue temperature to a depth of three centimeters.

Figures 1, 2, 3 and 4 demonstrate changes in tissue temperature at various depths with application of either shortwave diathermy, ultrasound, or hot packs^{13 15}.

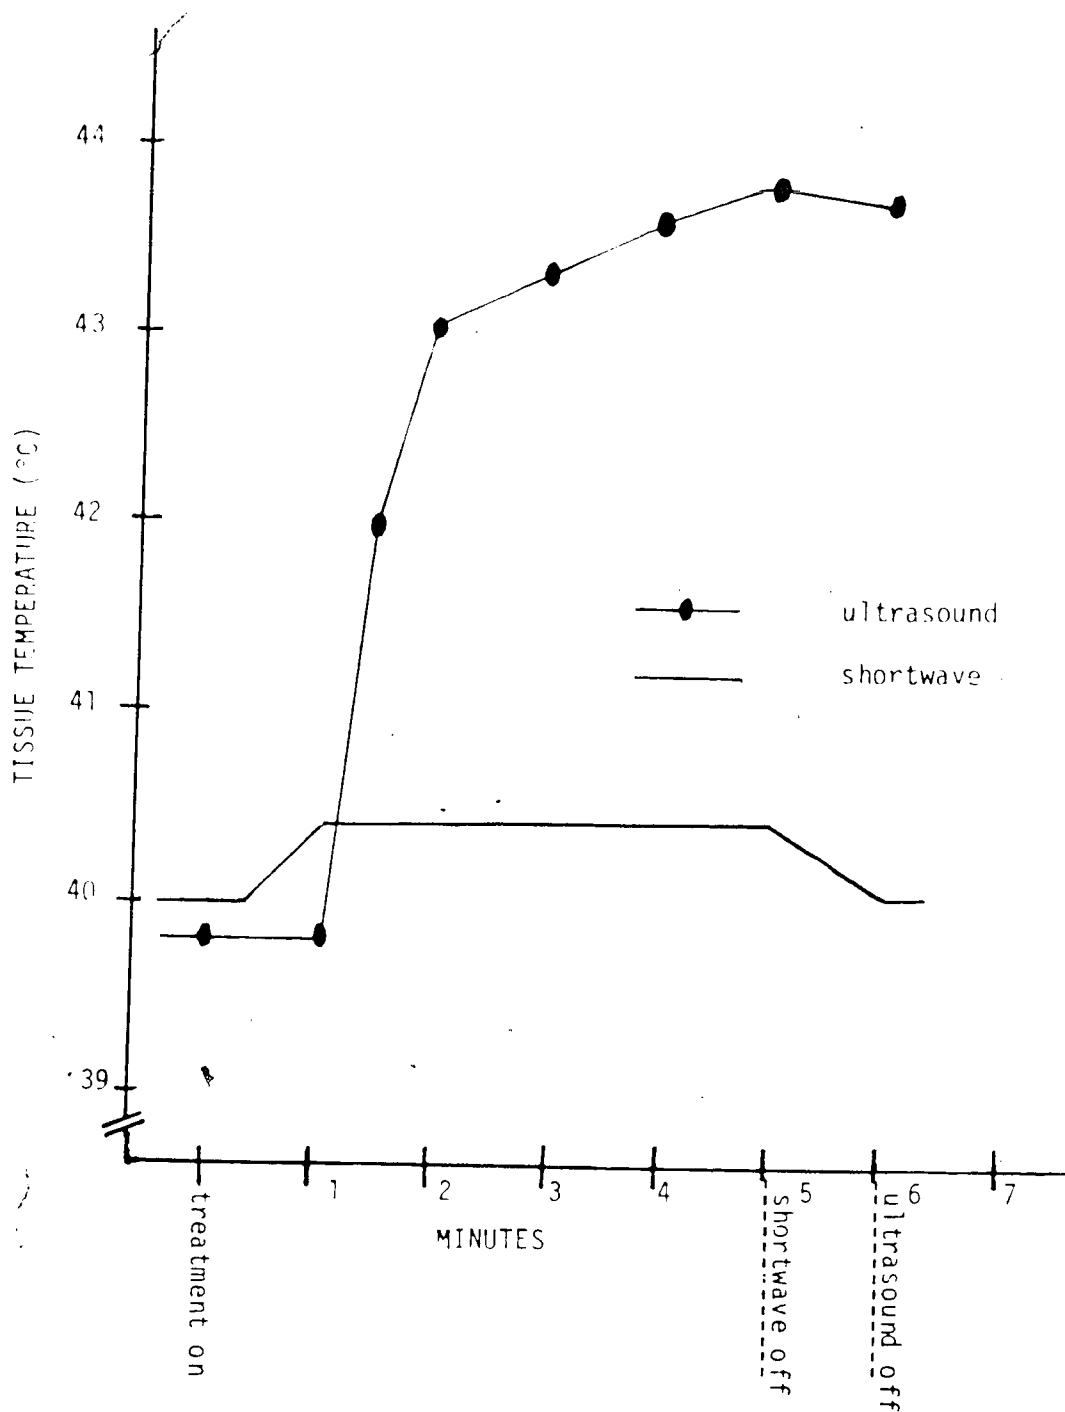


FIGURE 1: CHANGE IN TEMPERATURE INSIDE THE HIP JOINT FOLLOWING THE APPLICATION OF SHORTWAVE DIATHERMY AND ULTRASOUND

Adapted from: Lehmann JT, ed: Therapeutic Heat and Cold. Williams and Wilkins. Baltimore/ London, 1982, pg. 495.

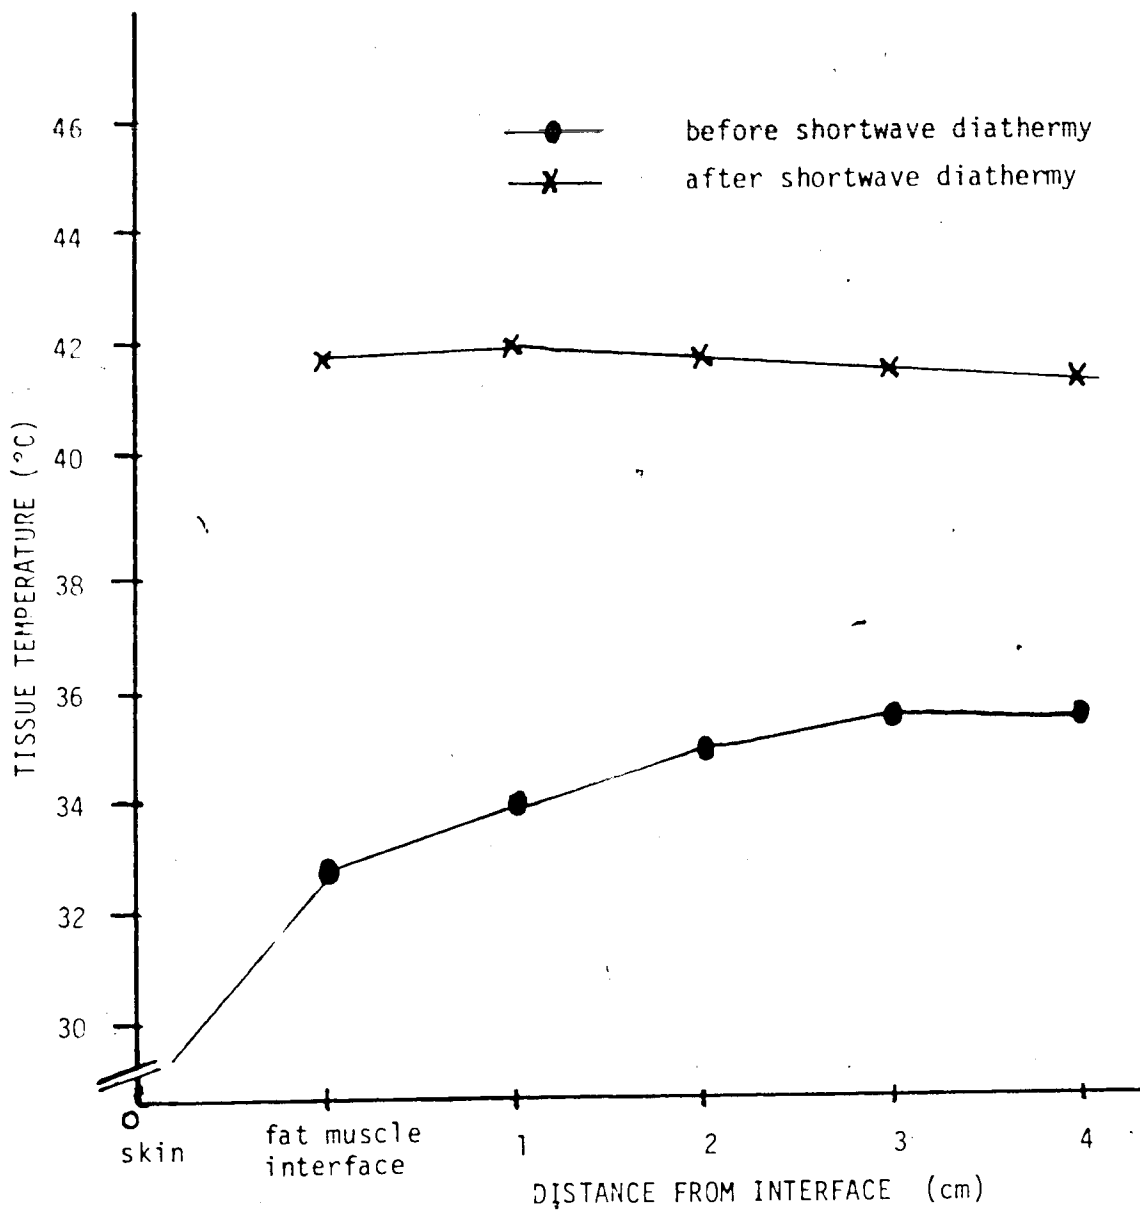


FIGURE 2: TEMPERATURE DISTRIBUTION IN THE HUMAN THIGH AT THE COMPLETION OF 20 MINUTES OF SHORTWAVE DIATHERMY

Adapted from: Lehmann JT, ed: Therapeutic Heat and Cold. Williams and Wilkins. Baltimore/ London, 1982, pg. 455.

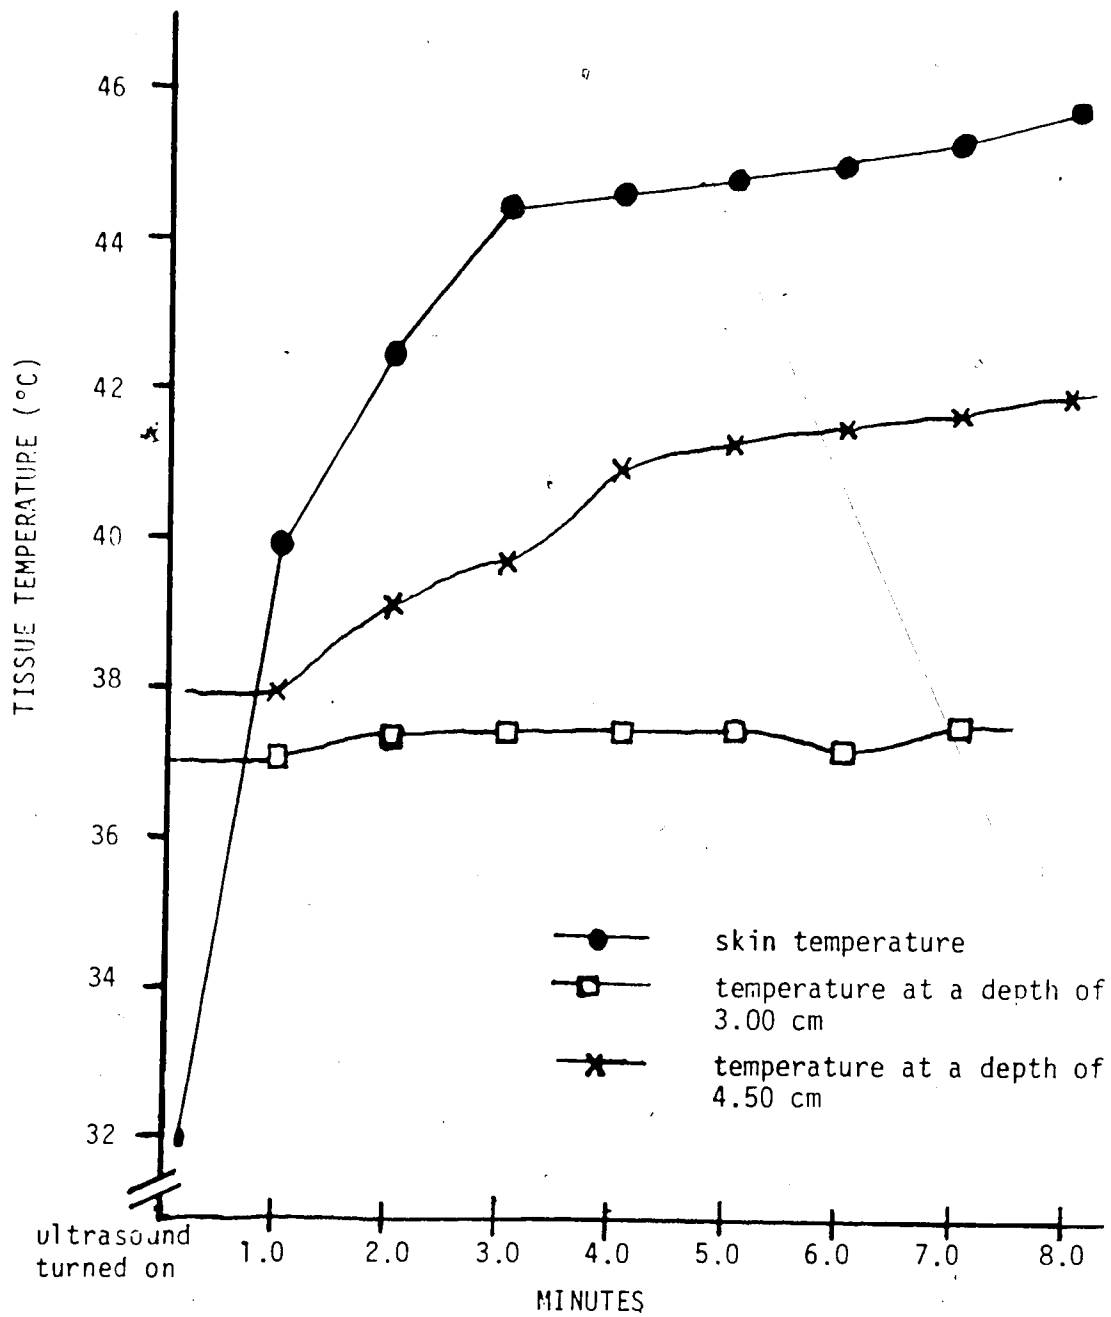


FIGURE 3: TISSUE TEMPERATURE CHANGE AT SKIN SURFACE 3.00 cm AND 4.5 cm DURING THE APPLICATION OF ULTRASOUND (INTENSITY: 1 wtt/cm²; MINERAL OIL COUPLE AT 24°C)

Adapted from: Lehmann JT, Delateur BJ, Selverman DH: Selective Heating Effects of Ultrasound in Human Beings. Arch Phys Med Rehabil 47:333, 1966.

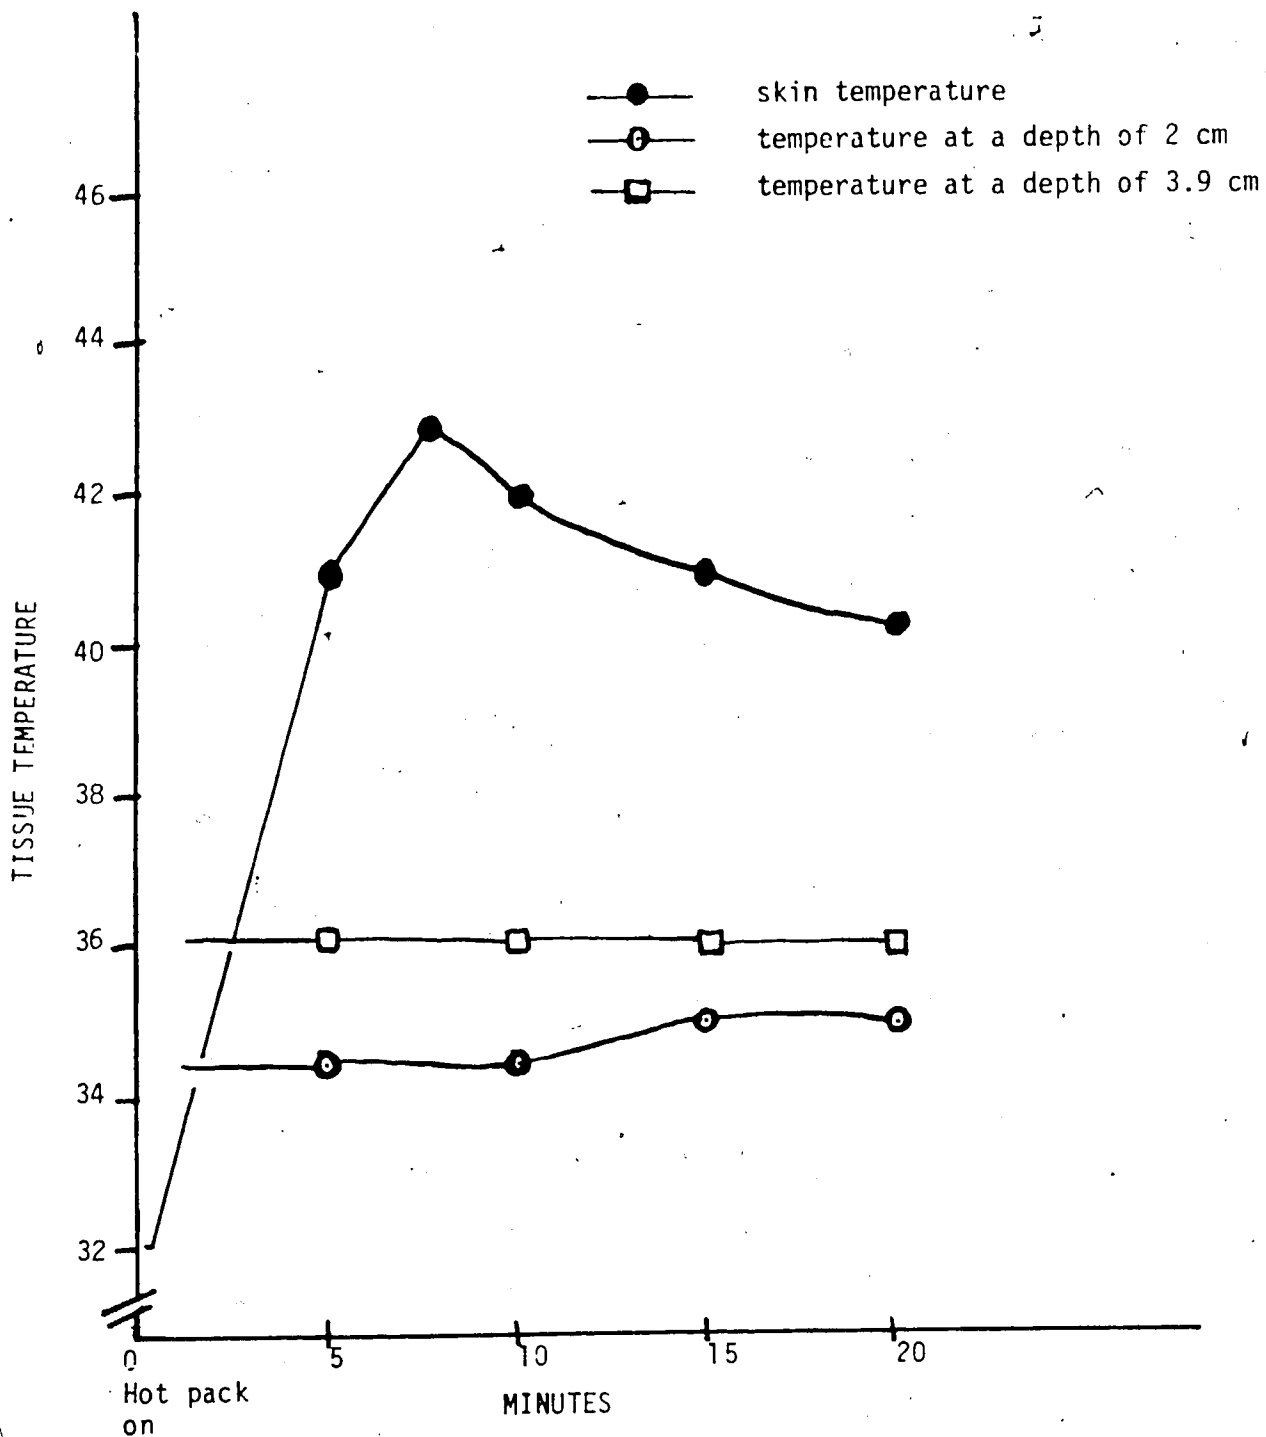


FIGURE 4: TISSUE TEMPERATURE CHANGE AT SKIN SURFACE, 2.0 and 3.9 cm DURING 20 MINUTES APPLICATION OF HOT PACK

Adapted from: Lehmann JT, ed: Therapeutic Heat and Cold. Williams and Wilkins. Baltimore/ London, 1982, pg. 430.

Tissue may either absorb or transmit heat differently depending on the modality used. Table 1 is a summary of the reaction of various tissues to the three different modalities¹¹.

TABLE 1

Comparison of the absorption and the transmission of shortwave diathermy, ultrasound, and hot packs in different body tissue.

Tissue	Modalities		
	Shortwave Diathermy	Ultrasound	Hot Packs
Fat	-high absorption -poor dissipation of heat	-low absorption, high transmission	-high absorption -poor dissipation of heat
Muscle	-high absorption, low transmission	-poor absorption -high transmission	-absorption if heat penetrates to muscle depth
Bone	-poor absorption -impede heat transfer	-high absorption may reflect ultrasound waves at bone-soft tissue interface	-does not penetrate to bone
Nerve	?	-high absorption, low transmission	?
Bone-muscle interface	?	-reflection of ultrasound causes local increase heat in adjacent tissue	?

Adapted from: Wadsworth H, Chanmugan A: Electrophysical Agents in Physiotherapy Therapeutics and Diagnostic Use. Science Press. Manichville NSW Australia, 1980. (? = unknown)

Because fatty tissue has a high absorption rate with shortwave diathermy and hot packs, and a low absorption rate with ultrasound, it might be presumed this difference in the absorption rate between the three modalities will have different effects on the heating of tissue lying below the fat.

To date, the question of the effects of shortwave diathermy, ultrasound, and hot packs on motor nerve conduction velocity has not been fully answered. Physical therapists utilize these modalities over peripheral nerves and nerve roots without knowing the physiological effects these modalities may have on the underlying nervous tissue. The frequency with which these modalities are used, for example, in the treatment of low back pain, makes it essential to understand their physiological effects.

RESEARCH HYPOTHESES

1. H₁: There is an increase in motor nerve conduction velocity following the application of shortwave diathermy, ultrasound or hot packs.
2. H₂: There is an increase in subcutaneous tissue temperature following application of shortwave diathermy, ultrasound or hot packs.
3. H₃: There is a significant correlation between the observed changes in motor nerve conduction velocity and the observed changes in subcutaneous tissue temperature following treatment with each of the three modalities.

OBJECTIVES

The objectives of the present investigation are:

1. Compare the effects of shortwave diathermy, ultrasound, and hot packs given at therapeutic dosage and applied in a manner consistent with procedures used clinically on: 1) the motor conduction velocity of the ulnar nerve, and 2) the local subcutaneous tissue temperature.
2. Examine the correlation between any observed changes in motor nerve conduction velocity and observed changes in tissue temperature.

OPERATIONAL DEFINITIONS

1. Therapeutic shortwave diathermy is a form of convective heat, utilizing an electromagnetic radio frequency of 27.12 megahertz with a wavelength of 11.06 meters. Monode inductothermy consists of a flat rigid cell encased in a perspex cover. Tissue heating occurs as a result of electromagnetic radiation producing an oscillation of the molecules within the field, and thereby heating the tissue^{11 15}.

2. Therapeutic ultrasound is a form of mechanical energy utilizing an acoustic vibration with a frequency of 870 kilohertz and an intensity of one watt per square centimeter. Tissue heating occurs as a result of longitudinal waves producing a vibration of particles within the acoustic field. It is the mechanical friction between the particles that produces heat^{11 15}.
3. Hot packs provide a form of conduction heat; passing from the warmer pack to the cooler tissue with which it is in contact. A hot pack contains silica gel and is covered by strong cloth. The silica gel is capable of absorbing many times its own volume of water and, when heated, to give off thirty to forty minutes of moist heat¹¹.

DELIMITATIONS

1. Only the ulnar nerve of the dominant arm was tested¹⁶.
2. The age range of the subjects was from 18 to 45 years. Both female and male subjects were examined¹⁶.
3. All subjects fell on or below the 80 percentile range for the minimum triceps skinfold thickness indicating obesity, as defined by Mayer¹⁸. As the subcutaneous fat layer is a critical factor when considering the selective tissue heating produced by shortwave diathermy, ultrasound, and hot packs, the delimitation as noted was necessary¹¹.

LIMITATIONS

1. As there are no standards for the minimum skinfold thickness indicating obesity in the forearm, that of the triceps was used, as it is the closest area having a standard^{17 18}.
2. The temperature probe was inserted into the subcutaneous fat layer. Its precise depth was not measured because the probe was inserted diagonally.
3. The consistency in selection of the same point of upward deflection of the baseline for the nerve conduction velocity determination was limited by the ability

of the investigator to consistently detect this point of deflection. See description of the reliability test, Appendix C.

D

{

7

REFERENCES - CHAPTER I

1. Gasser, HS: Nerve activity as modified by temperature changes. *Am J Physiol* 97:254-270, 1931.
2. Abramson DD, Bell Y, Rejal H: Changes in blood flow, oxygen uptake and tissue temperature produced by therapeutic agents: II effects of shortwave diathermy. *Am J Phys Med* 39:87-95, 1960.
3. Madsen PW, Gusten JW: The effects of ultrasound on conduction velocity of peripheral nerve. *Arch Phys Med Rehabil* 42:645-649, 1961.
4. Zankel HT: Effect of physical agents on motor nerve conduction velocity of the ulnar nerve. *Arch Phys Med Rehabil* 47:787-792, 1966.
5. Abramson PD, Chu LSW, Tuck S Jr, Lee SW, Richardson G, Levin M: Effect of tissue temperature and blood flow on motor nerve conduction. *JAMA* 198:1082-1088, 1966.
6. Farmer WC: Effect of intensity of ultrasound on conduction of motor axons. *Phy Ther* 48:1233-1237, 1968.
7. Currier DP, Nelson RM: Changes in motor nerve conduction velocity induced by exercise and diathermy. *Phy Ther* 49:146-152, 1969.
8. Halar EM, Delisa TA, Brozovich FV: Peroneal nerve conduction velocity: the importance of temperature correction. *Arch Phys Med Rehabil* 62:439-443, 1981.
9. Halle JS, Scoville CR, Greathouse DS: Ultrasound's effect on conduction latency of the superficial radial nerve in man. *Phy Ther* 61:345-350, 1981.
10. Licht S., ed: *Therapeutic Heat and Cold. Volume Two of Physical Medicine.* Waverly Press Inc., Baltimore, 1965.
11. Wadsworth H, Chanmugan A: *Electrophysical agents in physiotherapy: therapeutic and diagnostic use.* Science Press, Manichville NSW Australia, 1980.
12. Griffin JE: Physiological effects of ultrasound energy as it is used clinically. *J Am Phy Ther* 46:18-26, 1966.
13. Lehmann JT, DeLateur BJ, Silverman DH: Selective heating effects of ultrasound in human beings. *Arch Phys Med Rehabil* 47:331-339, 1966.
14. Lehmann JT, Silverman DR, Baum BA, Kirk NL, Johnston VC: Temperature

- distribution in the human thigh produced by infrared, hot pack, and microwave applications. Arch Phys Med Rehabil 47:291-299, 1966.
15. Lehmann JT, ed: Therapeutic Heat and Cold. Williams and Wilkins. Baltimore, 1982.
 16. LaFratta CW, Smith OH: A study of the relationship of motor nerve conduction velocity in the adult to age, sex and handedness. Arch Phys Med 43:407-412, 1964.
 17. Mayer J: Overweight: causes, costs and control. Prentice Hall Inc., Englewood Cliffs, New Jersey, 1968.
 18. Larson LA, ed: International Committee for Standardization of Physical Fitness Tests. MacMillan Publishing Company Inc., New York, 1974.

B. CHAPTER II - REVIEW OF THE LITERATURE

Shortwave diathermy, ultrasound, and hot packs each have a unique tissue heating effect^{1, 2}. As a result, evaluation of each modality is essential to determine the selective effect each modality may have on conduction velocity of a motor nerve.

SHORTWAVE DIATHERMY

Inductothermy is a method of shortwave diathermy in which an electromagnetic field is set up around the loops of a coil through which a current is passing. The electromagnetic field is more concentrated near the conductor and will heat the more superficial tissue¹. The production of heat is brought about by the friction of the tissue particles produced by the oscillation of the currents¹.

Inductive shortwave diathermy selectively heats tissue with the highest vascular content (i.e., muscle) and the lowest electrical impedance before heating tissue with a lower vascular content³. The greatest increase of tissue heat occurs in the area of the greatest current density³.

The depth of penetration of heat is inversely proportional to the thickness of the subcutaneous fat layer^{4, 5}. Lehmann, et al⁴ found an increase in tissue temperature at a depth of 3.89 centimeters following a 20 minute application of shortwave diathermy.

Literature concerning the effects of shortwave diathermy on motor nerve conduction velocity is limited. Currier⁶ studied the effects of reflex heating of the peroneal nerve by a 20 minute drum application of shortwave diathermy to the lumbosacral area. Direct heating of the lumbosacral area produced an increase in skin temperature to 45.5 degrees Celsius, whereas the indirect heating of the skin over the peroneal nerve in the leg produced an increase in temperature to 30.54 degrees Celsius. As a result of this indirect heating, there was a small increase of 0.24 degrees Celsius in the skin temperature over the peroneal nerve and a non-statistically significant increase in motor nerve conduction velocity. The author postulated that the reason for such a small increase in motor nerve conduction velocity was that the reaction of increased tissue heat was smaller with indirect heating than the reaction to direct heating. As there was only a minor heating of the peroneal nerve by this method, this minor increase in temperature of the skin over the peroneal nerve accounts for the non-statistically significant rise in the

conduction velocity of the peroneal nerve.

Abramson, et al.⁷ investigated the effects of shortwave diathermy (conductive) on motor nerve conduction velocity by placing one air spaced plate electrode over the shoulder and arm and the other over the wrist and hand. In addition, a six inch segment of the forearm was placed in a plethysmograph at different water temperatures: 34 and four degrees Celsius. In this manner, it was possible to compare the effects of shortwave diathermy on motor nerve conduction velocity when the forearm was warmed or cooled. Shortwave diathermy given for 25 minutes with a water temperature of four degrees Celsius produced a much greater increase in skin, subcutaneous tissue and muscle temperature as well as an increase in motor nerve conduction velocity of both the ulnar and median nerves than did the same procedure at 34 degrees Celsius. Two possible explanations were given. Firstly, the greater rise in tissue temperature and motor nerve conduction velocity observed at lower bath temperature may have been due to the ineffective removal of heat as a result of the vasoconstriction of the blood vessels caused by the cold water. A second possibility was these subjects were able to tolerate a greater degrees of shortwave diathermy without experiencing pain than those who had the higher water temperature. The authors concluded that an increase in tissue temperature by the above method could cause an increase in motor nerve conduction velocity of the ulnar and median nerves.

ULTRASOUND

Griffen⁸ has stated four possibilities that may occur when ultrasound is applied to tissue. It may be absorbed, transmitted, reflected, or refracted. Absorption is dependent mainly on the protein content of the tissue. There is an inverse relationship between absorption and penetration in any given tissue. Nervous tissue is second only to bone in its capacity to absorb ultrasound. Peripheral nerves absorb twice as much ultrasound as skeletal muscle, and skeletal muscle absorbs more ultrasound than fat¹. As it is the absorption of ultrasound that produces heat, it can be seen that bone is selectively heated most, then nervous tissue, whereas ultrasound will have a relatively low heating effect on fat¹.

The penetration of ultrasound is dependent upon the frequency used. The lower the frequency, the greater the depth of penetration⁸. For example, at a frequency of 90 kilohertz, 50 percent of the ultrasound energy will penetrate to a depth of ten centimeters, whereas, when ultrasound is applied over the same site, given at a frequency of one megacycle, 50 percent of the ultrasonic energy will penetrate to a depth of five centimeters⁸.

The net increase in temperature brought about by ultrasound is dependent on the intensity, the area exposed, and the duration of the treatment. The higher the intensity, the greater is the heat production⁹. Lehmann⁹ suggested that an area between two to five square inches (12.9 to 32.3 square centimeters) should be treated at one time. He reasoned that by moving the ultrasound head within this area, a uniform heating of the area would result. Also, if the size of the area is increased, then an increase in tissue temperature could not be expected as the heat was dissipated from the exposed area faster than it is put into it⁹.

Oakley¹⁰ suggested that if the area to be treated is larger than one and one half times the transducer head, the site should be divided into sections, each about one and one half the size of the transducer head and each section treated individually. By doing this, a uniform treatment over the area is ensured as well as prevention of concentration of peak intensities. These principles must be taken into consideration when reviewing the literature concerning the effects of ultrasound on motor nerve conduction velocity.

Zankel¹¹ studied the effects of ultrasound using two different methods. First, the ulnar nerve at the elbow was sonated for five minutes, and motor nerve conduction velocity from the axilla to the wrist was measured. In the second procedure, ultrasound was applied at different intensities and various durations to the ulnar nerve along its course in the forearm, and motor nerve conduction velocity was measured from the elbow to the wrist. In both procedures, only skin temperature was recorded. Procedure one did not produce a change in conduction velocity of the ulnar nerve at either one or two watts per square centimeter. In procedure two, the different intensities and duration (i.e., one watt per square centimeter for five minutes, and ten minutes, as well as two watts per square centimeter for five minutes) produced a decrease in motor nerve conduction velocity of the ulnar nerve. There was no statistically significant change in skin

temperature after the application of the ultrasound in either procedure. Despite this fact, the author concluded that the decrease seen in motor nerve conduction velocity of the ulnar nerve could be explained by some effect of ultrasound other than heat production. He felt that this decrease in motor nerve conduction velocity may have been due to a change in the rate of exchange of transmembranal electrolytes caused by the stirring or micromassage of the ultrasound. Zankel did not address the possibility that the area of exposure might have been too large with respect to the time duration to allow for effective tissue heating. Certainly, the area exposed was much greater than that suggested by Lehmann³ or Oakley¹⁶. The immediate cooling effect of the ultrasonic gel was another factor not considered¹.

Farmer¹² studied the effects of ultrasound at a frequency of 87 megahertz at various intensities, (0.5, 1.5, two, and three watts per square centimeter) by sonating the ulnar nerve from the elbow to the wrist for five minutes. Changes in tissue temperature were not recorded. Farmer reported an increase in motor nerve conduction velocity at 0.5 and three watts per square centimeter and a decrease in motor nerve conduction velocity at one, 1.5, and two watts per square centimeter. Farmer reasoned that the mechanical effects overpowered the thermal effects of ultrasound at one, 1.5 and two watts per squared centimeter resulting in a decrease in motor nerve conduction velocity, whereas the thermal effects at 0.5 and three watts per square centimeter produced an increase in the motor nerve conduction velocity of the ulnar nerve.

Madsen and Gersten¹³ demonstrated the importance of the relationship between ultrasound intensity, area exposed and duration of exposure. The frequency used in the study was one megahertz for each of two ultrasound generators, one having a sound head area of seven square centimeters, the other having a sound area of 12 square centimeters. The area exposed to ultrasound was the ulnar nerve from the elbow to the wrist for five minutes. This area was far greater than that suggested by Lehmann³ or Oakley¹⁶.

Application of ultrasound with a crystal head size of 12 square centimeters at an intensity of 0.88 and 1.28 watts pers square centimeter produced a statistically significant decrease in motor nerve conduction velocity of the ulnar nerve, while 1.92 watts per square centimeter produced a 0.5 degrees Celsius increase in tissue

temperature and an increase in motor nerve conduction velocity of the ulnar nerve. Madsen et al. also compared the different tissue temperature changes produced by both ultrasound generators used at various intensities. He reported a consistently greater increase in tissue temperature with the larger sound head at any given intensity. When the authors decreased the area covered by the sound head by half, both the temperature rise in the subcutaneous tissue and the motor nerve conduction velocity of the ulnar nerve doubled! Giving a mock ultrasound application (i.e., no emission of energy) resulted in a decrease in both tissue temperature and motor nerve conduction velocity of the ulnar nerve. Although the authors did not give a reason, it is possible that the cooling effect of the coupling agent was responsible for the decrease seen in the motor nerve conduction velocity⁷.

Esmat¹⁴, using the same procedure of sonating the ulnar nerve in the forearm as described in the previous studies, reported intensities of 0.5 and one watt per square centimeter to be the most effective in producing an increase in motor nerve conduction velocity of the ulnar nerve. At an intensity of two watts per square centimeter, no significant increase in ulnar nerve conduction velocity was observed. However, when the ultrasound was given in a water bath at a temperature between 33 and 35 degrees Celsius there was a decrease in conduction velocity. The author did not discuss any possibilities that might explain this finding.

From the above articles, it can be seen that disagreement exists in the literature regarding the effects of ultrasound on motor nerve conduction velocity. Three studies^{11, 12, 13} reported a decrease at lower ultrasound intensities, whereas one study¹⁴ reported an increase at similar levels.

HOT PACKS

Hot packs do not have a selective tissue heating effect. Tissue heating is produced by a conductive heat transfer from the hot pack to the cooler underlying skin⁵. Therefore, hot packs predominantly heat the superficial tissue rather than the deep tissue. Hot packs are capable of producing an increase of five degrees Celsius in the temperature of the skin beneath the hot pack¹⁵. Lehmann, et al.¹⁵ demonstrated that hot packs are capable of producing an increase in tissue temperature to a depth of three centimeters.

However, the authors demonstrated a slight increase of two degrees Celsius in tissue temperature at a depth of two centimeters after a twenty minute application of hot packs¹⁵.

Information on the effects of hot pack on motor nerve conduction velocity is scant. Zankel¹¹ reported that hot packs applied to the ulnar nerve region at the elbow for thirty minutes produced an increase in skin temperature of 9.5 degrees Fahrenheit (12.5 degrees Celsius) and a slight rise in motor nerve conduction velocity of the ulnar nerve. It is the large myelinated type A fibers that are the "motor nerve" part of peripheral nerve. It is from these large myelinated type A fibers that the motor nerve conduction velocity is tested¹⁷.

NERVE CONDUCTION VELOCITY

The range of normal motor nerve conduction velocity of the ulnar nerve is from 46 to 75 meters per second with the mean of 59.8 meters per second^{16, 17}. It is the large myelinated type A fibers that are the "motor nerve" part of a peripheral nerve. It is from these large myelinated type A fibers that the motor nerve conduction velocity is tested.¹⁷

In the adult, age has no effect on motor nerve conduction velocity until the age of 60 years. After the age of 60 years there is a slight decrease in the conduction velocity of motor nerves^{18, 19}. LaFratta, et al¹⁹ believe that this decrease in motor nerve conduction velocity has no clinical significance.

NEUROPHYSIOLOGICAL MECHANISM OF NERVE CONDUCTION

Conduction velocity is the distance an electrical impulse travels along a nerve fiber per unit of time²⁰. A peripheral nerve is made up of many thousands of nerve fibers, of which there are three basic types^{20, 21}. Type A nerve fibers are the largest in diameter (12-22 millimicrons) and the fastest in conduction (30-120 meters per second). They are myelinated and are somatic afferent and efferent nerve fibers. Type B nerve fibers are smaller (5 - 12 millimicrons) and slower (30-60 meters per second) and are also myelinated. These fibers are efferent preganglionic fibers of the autonomic nervous system. Type C are unmyelinated fibers that are smaller (0.5 - 0.1 millimicrons) and slower (0.5 - 30 meters per second) and are associated with pain sensation²⁰.

In the resting state, the nerve fiber is charged; that is there is a difference in the electrical potential between the interstitial fluid outside the nerve fiber and the intracellular fluid inside the nerve fiber²⁰. This resting membrane potential is usually between -70 and -90 millivolts and is generated by the sodium potassium pump. This ionic pump maintains a high concentration of sodium and chloride ions in the interstitial fluid outside the nerve fiber and a high concentration of potassium ions in the intracellular fluid within the nerve fiber. The resting membrane is relatively impermeable to sodium ions; therefore there is very little leakage of sodium into the nerve fiber²¹. Potassium ions diffuse through the nerve fiber membranes more easily, and tend to leak out of the nerve fiber until an equilibrium is reached when the inside of the nerve fiber reaches an electrically negative potential relative to the interstitial fluid (-70 to -90 millivolts). When an electrical stimulus of sufficient intensity stimulates a nerve fiber, it produces an action potential which is then self propagating^{20 21}. The action potential is characterized by the following sequence of specific events: depolarization of the nerve fiber membranes; change of permeability of the nerve fiber membrane resulting in an influx of sodium ions into the intracellular space, a momentary reversal of the resting membrane potential; inactivation of the mechanism responsible for the increase in permeability of the membrane to sodium; and, an increase of permeability of the nerve fiber membrane to potassium which results in an efflux of potassium ions out of the nerve fiber returning the membrane potential to its resting state^{20 21 22}. Depolarization of the nerve fiber is best seen when a sub-threshold stimulus (a stimulus that is not strong enough to produce an action potential) is applied to a nerve fiber. A weak sub-threshold stimulus applied to the nerve fiber causes a redistribution of ions across the nerve fiber membrane which reduces the membrane potential. If the stimulus strength is increased, this redistribution of ions across the nerve fiber membrane is increased, and, if the threshold level is reached, an action potential develops explosively and is thereafter independent of the stimulus²¹. Once the action potential is initiated, the membrane at that point becomes freely permeable to sodium ions allowing an influx of sodium ions into the nerve fiber at that particular site. As the result of the sodium ion influx, the membrane potential is reversed (to about +40 millivolts). Inactivation of the sodium influx is brought about by a decrease in sodium conductance. Even while inactivation of sodium ions is occurring, there is an efflux of potassium ions out of the

nerve fiber. This potassium ion efflux helps to restore the membrane back to its original resting state²¹. The self propagation of an action potential occurs by a process referred to as local circuit propagation²¹. Local circuit propagation is brought about by a potential difference between two adjacent regions of the nerve fiber. At one site (where the action potential is occurring), the membrane potential is near the sodium equilibrium potential (around +40 millivolts) and adjacent to this site, the membrane potential is near the potassium equilibrium potential (around -80 millivolts). Thus, there is a potential difference between these two adjacent regions. As a result of this potential difference, a local circuit current flows from the active region through the intracellular region to the inactive region producing a decrease in the membrane potential at the inactive region. When the membrane potential is decreased to threshold level, the permeability to sodium increases rapidly and an action potential occurs. In this way, local circuit currents produced by sodium influx and potassium efflux at an "active" region stimulates the adjacent "inactive" regions which then become "active" and an action potential is propagated along the nerve²¹.

This basic summary of the neurophysiological mechanism of nerve conduction is helpful in understanding the review of the literature on how heat causes an increase in nerve conduction. Hodgkin, Huxley and Katz²³ found that a rise of 16 degrees Celsius in the squid axon resulted in a six-fold increase in the rate at which the ionic currents changed. This increase in temperature predominately increased the rate of efflux of the potassium and, to a lesser extent, the rate of the influx of sodium ions. In an earlier study, Hodgkin and Katz²⁴ found that temperatures between three and 20 degrees Celsius had little effect on the resting membrane potential of the squid axon. However, temperatures above 20 degrees Celsius reduced the resting potential, and temperatures below 3 degrees Celsius resulted in a slowing of the action potential particularly of the declining phase of the action potential. That is, below 3 degrees Celsius, it took longer for the potassium efflux to occur. The authors postulated that a rise in temperature might affect the permeability of sodium ions. They believed that the transfer of sodium through the cell membrane was governed by a special process involving a transient reaction with the membrane molecules and that this transient reaction had a higher temperature coefficient than the migration of potassium or chloride ions through the nerve membrane. Work

done by Gasser²⁵, and Schoepfle and Erlanger²⁶, agreed with the above findings of Hodgkin, Huxley and Katz. Gasser²⁵ compared the rate of change of the potential in each part of the action potential in frog nerve at 24 and 12 degrees Celsius. He found that at the lower temperature (12 degrees Celsius), there was a decrease in the rate of change of the action potential. He postulated that the change in temperature might affect the viscosity of the axon cytoplasm. An increase in viscosity (caused by a lowering of temperature) would interfere with the development of the action potential and would prolong the recovery process of the axon back to its resting potential. Schoepfle, et al.²⁶ found that cooling the nerve to between eight and nine degrees Celsius resulted in a prolongation of the descent part of the action potential and consequently increased the area of the action potential. They also found that when the nerve was cooled, there was a slight increase in the time it took for the appearance of the action potential to begin after the stimulus was given.

In summary, it seems that heating nerves results in an increase in nerve conduction velocity by one or a combination of the following:

1. Heat increases the sodium influx and the potassium efflux.
2. Heat increases the nerve membrane permeability to the migration of sodium ions.
3. Heat decreases the viscosity of the axon cytoplasm and therefore movement of ions within this cytoplasm is easier.
4. Heat lowers the resting membrane potential of the nerve fiber at higher temperatures.

CONCLUSION

Despite the heat effects produced by shortwave diathermy, ultrasound, and hot packs, these modalities do not unconditionally cause an increase in motor nerve conduction velocity. The effect of different methods of application on the penetration of heat, and rise in temperature are two of the major variables to be considered. The duration of exposure and the tissue being heated must also be considered. The absorption coefficient of different tissues vary with the modality used. For example, the absorption coefficient of muscle is high when using shortwave diathermy and low when using ultrasound. The subcutaneous fat layer has a high resistance to the transmission of shortwave diathermy through to the deeper underlying tissue; whereas there is little

resistance occurring to the transmission of the ultrasound waves in fat tissue, allowing for easy transmission of the ultrasound through to the deeper tissue^{1 2 3}. It is evident that in comparing the effects of shortwave diathermy, ultrasound, and hot packs on motor nerve conduction velocity, the thickness of the subcutaneous fat layer is of importance. It is for this reason that the subcutaneous skin fold thickness was measured.

REFERENCES - CHAPTER II

1. Wadsworth H, Chanmuga A: *Electrophysical Agents in Diagnostic Physiotherapy: Therapeutic and Diagnostic Use*. Science Press. Manichville NSW Australia, 1980.
2. Lehmann JT, ed: *Therapeutic Heat and Cold*. Williams and Wilkins. Baltimore, 1982.
3. Licht S, ed: *Therapeutic Heat and Cold*. Volume Two of *Physical Medicine*. Waverly Press Inc., Baltimore, 1965.
4. Lehmann JT, DeLateur BJ, and Stonebridge JB: Selective muscle heating by shortwave diathermy with a helical coil. *Arch Phys Med* 50:117-123, 1969.
5. Hovind H and Nielsen SL: Local blood flow after shortwave diathermy: preliminary report. *Arch Phys Med* 55:217-221, 1974.
6. Currier DP and Nelson RM: Changes in motor conduction velocity induced by exercise and diathermy. *Phy Ther* 49:146-152, 1969.
7. Abramson DI, Chu LSW, Tuch S Jr, Lee SW, Richardson G, and Levin M: Effect of tissue temperature and blood flow on motor nerve conduction. *JAMA* 198:1082-1088, 1966.
8. Griffin JE: Physiological effects of ultrasonic energy as it is used clinically. *Phy Ther* 46:18-26, 1966.
9. Janis P: Ultrasound: the dosage question. *Physio Canada* 21:155-159, 1969.
10. Oakley EM: Application of continuous beam ultrasound at therapeutic levels. *Physiotherapy* 64:169-172, 1978.
11. Zankel HT: Effect of physical agents on motor nerve conduction velocity of the ulnar nerve. *Arch Phys Med* 47:787-792, 1966.
12. Farmer WC: Effect of intensity of ultrasound on conduction of motor axons. *Phy Ther* 48:1233-1237, 1968.
13. Madsen PW and Gersten JW: The effects of ultrasound on conduction velocity of peripheral nerve. *Arch Phys Med* 42:645-649, 1961.
14. Esmat N: Investigations on the effects of different doses of ultrasonic waves on

- the human nerve conduction velocity. *J Egypt Med Assoc* 58:395-402, 1975.
15. Lehmann JT, Silverman DR, Baum BA, Kirk ML, and Johnston VC: Temperature distribution in the human thigh produced by infrared, hot pack and microwave applications. *Arch Phys Med Rehabil* 47:291-299, 1966.
 16. Checklés NS, Russakov AD, and Prero DL: Ulnar nerve conduction velocity - effect of elbow position on measurement. *Arch Phys Med Rehabil* 52:362-365, 1971.
 17. Smorto MP and Basmajian JV: *Electrodiagnosis*. Harper Row Publishers. New York, 1977.
 18. Wagman IH and Lease H: Maximum conduction velocities of motor fibers of ulnar nerve in human subjects of various ages and sizes. *J Neurophysiol* 14-15:235-24, 1951-52.
 19. LaFratta CW and Smith OH: A study of the relationship of motor nerve conduction velocity in the adult to age, sex and handedness. *Arch Phys Med Rehabil* 45:407-412, 1964.
 20. Smorto MP and Basmajian JV: *Clinical Electroneurography*. The Williams and Wilkins Co. Baltimore, 1979.
 21. Ruch TC and Patton HD: *Physiology and Biophysics*. W.B. Saunders Co. Philadelphia, 1965.
 22. Keele, CA and Neil, E., eds.: *Samson Wright's Applied Physiology*. Eleventh Edition. Oxford University Press. Toronto, 1965.
 23. Hodgkin AG, Huxley AF, Katz B: Measurement of Current Voltage Relations in Membrane of the Giant-Axon of *Loligo*. *J Physiol* 116:424-448, 1952.
 24. Hodgkin AL, Katz B: The Effect of Temperature on the Electrical Activity of the Giant Axon of the Squid. *J Physiol* 109:240-249, 1949.
 25. Gasser HS: Nerve Activity as Modified by Temperature Changes. *Am J Physiol* 97:254-270, 1931.
 26. Schoepfle GM and Erlander J: The Action of Temperature on the Excitability Spike Height and Configuration, and the Refractory Period Observed in the Response of Single Modulated Nerve Fiber. *Am J Physiol* 134:694-704, 1941.

C. CHAPTER III - METHODS AND PROCEDURES

EXPERIMENTAL SUBJECTS AND EQUIPMENT

Subjects

Eighteen informed subjects were examined during repeated testing in six different treatment sequences as shown below. ¹ These six treatment sequences constituted all possible sequences of applying the three treatment modalities to the subjects in this experiment. By using these six different treatment sequences, control for any treatment effect and treatment order effect was achieved. Table 2 demonstrates the treatment sequence to which each subject was assigned. The method of repeated measurement was chosen to help control for the individual differences¹. The age range of the subjects was from 18 to 45 years². This age range was chosen to eliminate age as a factor affecting motor nerve conduction velocities. It has been reported there is a decrease in motor nerve conduction velocity after the age of 60 years².

A 10-12 centimeter segment of the anteromedial aspect of the forearm of the dominant arm of each subject was tested³. There is controversy in the literature as to whether there is a difference in motor nerve conduction velocity between the dominant and the non-dominant arm^{2 3}. By testing only the dominant arm, any variation of motor nerve conduction velocity between the dominant and the non-dominant arm that might occur was excluded.

A skinfold measurement of the triceps as described by Mayer⁴ and Larson⁵ was taken. Only those persons tested who fell within the 80 percentile range of minimum triceps skinfold thickness indicating obesity were accepted into the study. See Table 3 for the minimum triceps skinfold thickness indicating obesity for the age range of 18 to 45 years⁴.

All subjects were questioned regarding any history of upper or lower motor neuron disease, history of trauma to the ulnar nerve resulting in neuropraxia, axontmesis.

¹Sequence 1 - shortwave diathermy, ultrasound, hot pack
Sequence 2 - shortwave diathermy, hot pack, ultrasound
Sequence 3 - ultrasound, shortwave diathermy, hot pack
Sequence 4 - ultrasound, hot pack, shortwave diathermy
Sequence 5 - hot pack, ultrasound, shortwave diathermy
Sequence 6 - hot pack, shortwave diathermy, ultrasound

or neurotmesis, history of fracture or dislocation of the elbow of the dominant arm or history of peripheral vascular disease⁶. In addition, all persons were screened for diabetes and metal implants before being accepted into the study⁷. (see appendix A for Questionnaire for Screening Potential Subjects). All subjects were given an information sheet and were asked to sign a consent form (see appendix A).

As variation of room temperature may have an effect on motor nerve conduction velocity, the temperature of the laboratory was kept constant at 25 degrees Celsius, plus or minus 2 degrees.

Table 2
Assignment of Treatment Sequences to Subjects

Subject Number	Treatment Sequence
1	1
2	2
3	3
4	4
5	5
6	6
7	1
8	2
9	3
10	4
11	5
12	6
13	1
14	2
15	3
16	4
17	5
18	6

Table 3
Obesity Standards
Minimum triceps skinfold thickness indicating obesity (millimeters)

AGE (Years)	MALES	FEMALES
18	15	27
19	15	27
20	16	28
21	17	28
22	18	28
23	18	28
24	19	28
25	20	29
26	20	29
27	21	29
28	22	29
29	22	29
30-50	23	30

Reproduced from: Mayer J: Overweight: Causes, Costs and Control. Prentice-Hall Inc., Englewood Cliffs, New Jersey, 1968.

Position

All subjects were tested in a supine position with the dominant arm in approximately 60 degrees of abduction; 70 degrees of external rotation; and, 20 degrees of horizontal adduction of the shoulder. This position of the shoulder was chosen so as not to restrict blood flow to the arm. The elbow was flexed to approximately 90 degrees and the forearm fully supinated¹. This position was chosen in order to position the ulnar nerve laterally and uppermost and therefore make it easily accessible. The arm was stabilized in this position by pillows.

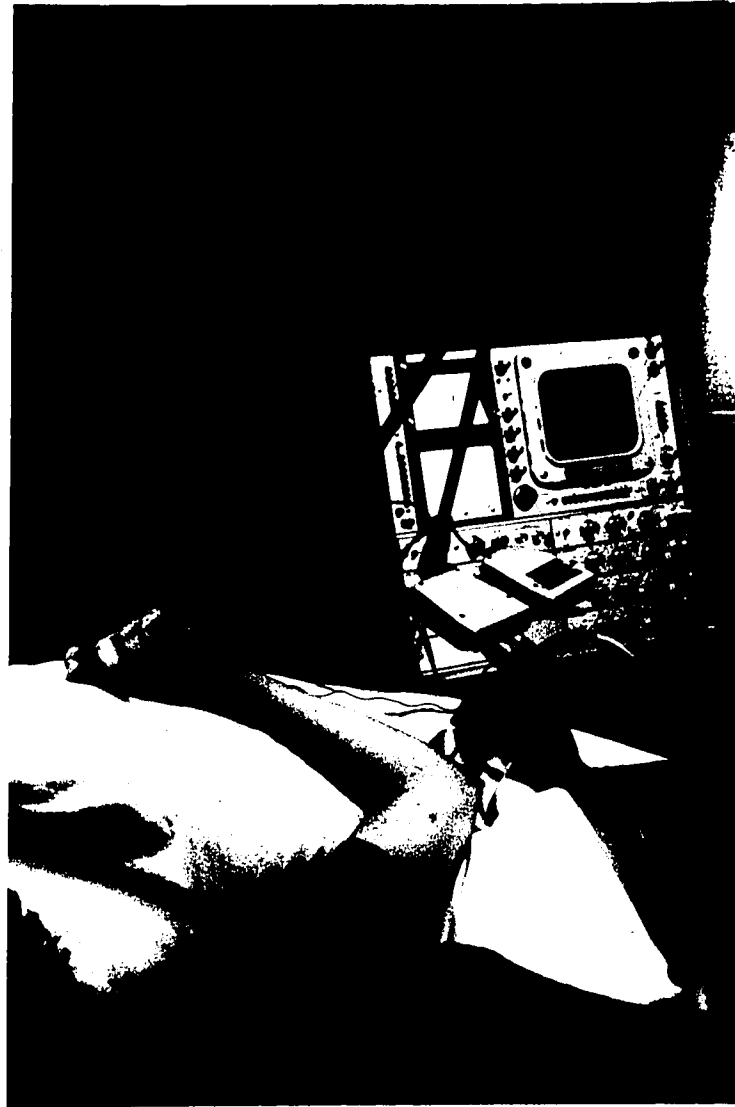


Figure 5

Position of the Subject During Experimental Procedure

Apparatus

1. Shortwave Diathermy

A Siemens 708 ultratherm with a frequency of 27.12 megahertz was used. An inductothermy monode with a diameter of nine centimeters was connected to the Siemens unit. The monode was placed three centimeters above the anteromedial aspect of the forearm, and centered directly over the inserted needle probe. The reason for this positioning was that inductothermy has a ring-shape heating pattern, heating the periphery more than the center of the ring¹¹. Therefore, by placing the center of the monode over the needle probe, selective heating of the needle probe was kept at a minimum. The duration of the shortwave diathermy treatment was 20 minutes. The intensity of the shortwave diathermy was such that the subject felt a comfortable warm heat.

2. Ultrasound

The ultrasound unit was a Burdeck model UT-420A which operated at a frequency of 870 kilohertz. The coupling agent used was aquasonic gel[®]. Intensity used was one watt per square centimeter. The current was continuous. The duration of treatment was five minutes. This intensity was chosen because it was within the therapeutic range of intensities used in a clinical setting.

3. Hot Pack

The hot pack used was a half size Tru-Moist Heat Pak (HP 151), Tru-Eze Manufacturing Company, kept in a hydrocollator with a water temperature of 70 degrees Celsius plus or minus five degrees Celsius⁷. The dimensions of the hot pack were 12 by 30 centimeters. The hot pack was covered by two layers of terry cloth hot pack covers. The hot pack and its covers were placed for a 20 minute period crosswise over the upper forearm. In this manner, a 12 centimeter segment of the forearm was heated by the hot pack. This procedure was chosen because it complied with the standard procedure followed in physical therapy departments and clinics.

4. Needle Probe and Digital Thermometer

Subcutaneous temperature was monitored by a 24 gauge needle probe Yellow Springs Instruments (YS 1) No24. The needle probes were gas autoclaved by the Department of Surgical Supply at the University of Alberta Hospital prior to each testing.

Subcutaneous temperature changes were recorded by a digital thermometer Model 49TA Yellow Springs Instruments for the ultrasound and the hot pack treatments. A scanning Tele-Thermometer Model 47 Yellow Springs Instruments was used to record subcutaneous temperature changes associated with the shortwave diathermy treatment. The reason the two different thermometers were used was that the battery-operated Yellow Springs 49TA thermometer had been found to be unduly sensitive to electromagnetic influence, whereas the electrically-operated Yellow Springs 47 thermometer had not. Therefore, as the scanning Tele-Thermometer was less affected by the electromagnetic current of the shortwave diathermy, this thermometer was used for recording the subcutaneous tissue temperature during the shortwave diathermy treatment.

5. Electromyograph

Nerve conduction velocity testing was performed using a TECA TE-42 Electromyograph. Permanent recordings were taken on TECA photographic paper.

6. Timer

All treatments during the experiment were timed by a Gra-lab Timer, model 171.

CALIBRATION OF EQUIPMENT

All the apparatus was calibrated (see Appendix B for details). To insure optimal internal validity, the same Siemens 708 monode, Burdick UT-420A, hot pack, needle probes, digital thermometer, scanning thermometer, electromyograph, timer and skinfold caliper were used throughout the experimental procedure.

A representative of Electromed Services calibrated the output of the shortwave diathermy unit by using a calibration light test box. The intensity of the ultrasound unit was

calibrated by a Russian ultraschalleisthngsmessgerat NMY-3 unit. Calibration of the hot pack was done by repeated measurement of the temperature of the bath water in the hydrocollator. This calibration was done over a period of three days. The bath water temperature had to remain at 70 degrees Celsius plus or minus five degrees Celsius. The needle probes were connected to the same digital thermometer and the same scanning thermometer for calibration. The same digital thermometer was used in each of the ultrasound and hot pack treatments and the same scanning thermometer was used in each of the shortwave diathermy-treatments. The two needle probes were calibrated against the same mercury thermometer and a temperature conversion scale for each needle probe to the chemical thermometer was made. All experimental procedures were timed by the same Gra-lab Timer. This procedure eliminated any discrepancies that may have existed between the timer on the shortwave machine and the ultrasound machine.

EXPERIMENTAL PROCEDURE

On arriving at the test laboratory, the subjects were given a full explanation of the testing procedures and then were asked to sign an Informed Consent Form (see Appendix A). Each subject was then assigned to one of the six treatment sequences as indicated in Table 2. There was a minimum of 48 hours between test procedures.

While standing, a triceps skinfold test was taken as described by Mayer³. In addition, a forearm skinfold test was taken in the following manner: once the proximal and distal stimulation points had been identified and marked, a point half-way between the two was marked and a skinfold thickness test was done at this site and recorded on the data sheet. The skinfold thickness test was taken with the crest of the skinfold in a longitudinal direction, parallel to the longitudinal axis of the forearm. Each subject was then asked to lie on a padded plinth and pillows were placed under their head and legs in order to make the subject comfortable. Their dominant arm was exposed from mid arm distally. The forearm and medial aspect of the hand was cleansed by rubbing it with isopropyl alcohol. The distal electromyographic electrode was placed over the muscle belly of abductor digiti minimi muscle and secured by tape. The ground electrode was placed on the tip of a finger. The stimulator was then placed over the ulnar nerve in the groove of the elbow. The position of the stimulator at which the greatest muscle action potential was seen on

the oscilloscope was marked with permanent ink. The course of the ulnar nerve was followed distally to where it emerged superficially in the mid forearm. The point of stimulation along the ulnar nerve at which the greatest muscle action potential was obtained (as detected on the oscilloscope) was marked with permanent ink. The distance between the proximal and distal stimulating sites was between 10-12 centimeters⁹.

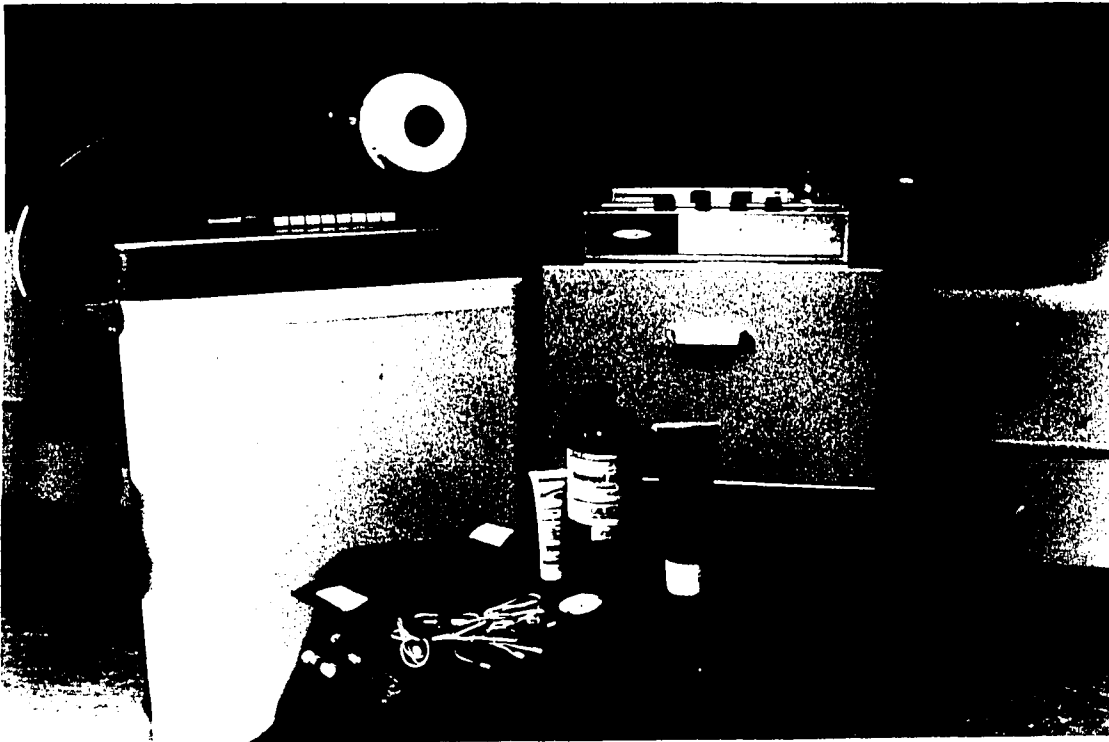


Figure 6

Equipment and Modalities Used in Experiment

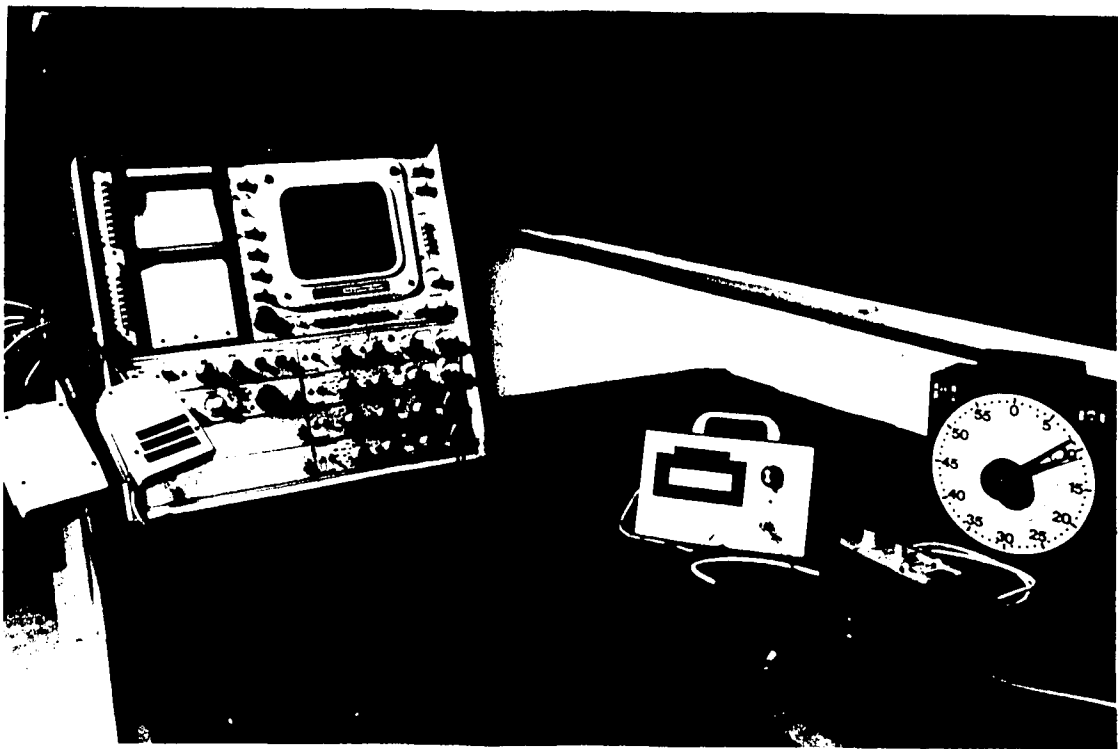


Figure 7

Electromyograph Timer, Digital Thermometer, Needle Probe, and Gra-lab Timer

The skin where the subcutaneous needle probe was to be inserted was cleansed by rubbing it with isopropyl alcohol. A subcutaneous needle probe was inserted by the experimenter to a length of approximately three centimeters diagonally into the subcutaneous tissue of the anteromedial aspect of the treatment arm half-way between the proximal and distal sites of stimulation¹⁰. The wire leading to the probe and the rubber tip of the probe was secured to the subject by tape in order to prevent pulling the probe out accidentally. The subject's temperature was allowed five minutes to stabilize. Stabilization was considered to have occurred when the subject's temperature had not fluctuated more than plus or minus 0.2 degrees Celsius over a period of one minute. Temperature recordings were taken at one minute pre-treatment, immediately prior to treatment (zero minute pre-treatment), and at one minute intervals during each of the treatments. Two other temperature recordings were taken: one immediately following the treatment (zero minute post-treatment), and the last recording was taken one minute after the end of the treatment procedure.

Immediately following the recording of the zero minute pre-treatment temperature, treatment was given in one of the following manners:

Shortwave diathermy

The application of shortwave diathermy followed the standard format used in a clinical setting.

A nine centimeter monode was placed three centimeters above the area to be treated. The monode was positioned (as stated previously) so that it was centered directly over the needle probe. The duration of the treatment was 20 minutes. The intensity was such that the subjects felt a comfortable warm heat. At the end of the treatment, the monode was removed and both the proximal and distal stimulation sites were wiped with dry gauze. This cleansing procedure was done in order to prevent any change in skin resistance that might have been caused by the accumulation of salt due to perspiration. Immediately after wiping the proximal and distal sites of stimulation, both the motor nerve conduction velocity and subcutaneous temperature were recorded. This procedure was repeated one minute later.

Ultrasound

The ultrasound intensity used was one watt per square centimeter with a frequency of 870 kilohertz applied for a duration of five minutes⁶. Aquasonic gel[®] served as the transmission medium. Overlapping circles at a rate of about two to three centimeters per second were used so that there was an even distribution of ultrasound energy. Full contact of the ultrasound head was maintained throughout treatment, in order to prevent loss of ultrasound energy⁶. Immediately following the end of the ultrasound treatment, the aquasonic gel[®] was removed at the proximal and distal sites of stimulation and a motor nerve conduction velocity test was completed and recorded as well as the subcutaneous temperature. The remaining aquasonic gel[®] was removed and a second motor nerve conduction velocity test and temperature were recorded one minute after the end of the treatment procedure.

Hot Pack

The hot pack was wrapped in two layers of terry cloth towelling and was applied to the anteromedial aspect of the forearm over the course of the ulnar nerve for a period of twenty minutes⁶. At the end of treatment, the hot pack was removed and both the proximal and distal stimulation sites were wiped clean with dry gauze. The cleansing procedure was done to prevent any change in skin resistance that might have been caused by the accumulation of salt due to perspiration. Immediately after wiping the proximal and distal sites of stimulation both the motor nerve conduction velocity and subcutaneous temperature were recorded. This procedure was repeated one minute later.

Motor Nerve Conduction Velocity

Motor nerve conduction velocity was tested by stimulating at both the proximal and distal points. A permanent record was taken of the supramaximal response by a foot control switch which took a picture of the electromyograph oscilloscope of fiber optic paper. Motor nerve conduction velocity data was collected at one minute pre-treatment, immediately prior to treatment, immediately following the end of the treatment, and one minute post-treatment.

Following the final temperature recording and motor nerve conduction velocity data recording, the needle probe was removed, the electrodes removed and the area cleaned.

Motor Nerve Conduction Velocity and Temperature Recordings

Four motor nerve conduction velocity recordings were taken. At one minute pre-treatment, zero minute pre-treatment, immediately at the end of treatment (zero minute post-treatment), and one minute after treatment ended. This same procedure was followed for temperature recordings. In addition to this, temperature recordings were made at one minute intervals during the five minute treatment of ultrasound and the twenty minute treatment of shortwave diathermy and hot pack.

STATISTICAL PROCEDURE

All statistical calculations were compiled by the University of Alberta Computing Services Statistical Application Analysis. Subcutaneous tissue temperature and motor nerve conduction velocity data were examined by a two by three way analysis of variance with repeated measurements over both factors⁶. A Neuman-Keuls multiple comparison of means was employed to compare selected means. The Pearson-Product Moment Correlation Coefficient was calculated for the one minute pre-treatment and the zero minute pre-treatment; and the zero minute post-treatment and the one minute post-treatment data for both subcutaneous tissue temperature and motor nerve conduction velocity. This calculation was done in order to test the examiner's reliability in testing motor nerve conduction velocity and to confirm that the subcutaneous tissue temperature had stabilized. The Pearson Product Moment Correlation Coefficient was calculated using all 18 subjects with three repeated measurements. The Pearson Product Moment Correlation Coefficient was also calculated for change in subcutaneous tissue temperature, change in motor nerve conduction velocity, and skinfold thickness layer for each modality taken separately.

Reliability Tests and Procedures

To ensure consistency in the experimental procedure, and maximize high internal validity, the following tests and procedures were performed (see appendix C for detailed description of each procedure).

1. Skinfold thickness test of the triceps and forearm.
2. Calculation of the motor nerve conduction velocity from the recordings made on the TECA photographic paper.

3. Control of experimenter's bias in calculation of the motor nerve conduction velocity.
4. The competency and safety of inserting a needle probe.

RISKS AND PRECAUTIONS

Burn is the most common potential risk to the subjects in the application of shortwave diathermy, ultrasound and hot packs. This risk factor was controlled and minimized by: 1) doing a skin sensation test to check the subject's discrimination between hot and cold; 2) wiping the skin dry of perspiration prior to the application of shortwave diathermy so as to prevent any point of concentration of the electromagnetic field on the skin; 3) by instructing the subject that they were to feel a comfortable, warm heat and NOTHING MORE. If they felt any discomfort whatsoever, they were to tell the experimenter and the machine would be turned off or the hot pack removed; 4) the subjects were under the constant supervision of the experimenter throughout the treatment procedure.

Contamination of the needle probe causing infection is a risk associated with the needle probe. This risk was controlled by having the needle probe gas autoclaved after each use. Further, the area of skin into which the needle has been inserted was first cleansed with isopropyl alcohol.

As the needle was inserted into an area where the ulnar nerve passes, there was a remote possibility that the needle might contact the ulnar nerve. This unlikely occurrence was minimized by holding the needle diagonally to the forearm, picking up in a pinch-type grasp the skin and the subcutaneous tissue into which the needle probe is inserted, and pushing the needle probe in a slow, steady motion through the subcutaneous tissue. In this way, if the needle probe did hit the fascia covering the muscle the resistance was felt by the experimenter, and the experimenter did not insert the needle any further. If one was sure not to pierce the muscular fascia this provided sure protection to the ulnar nerve since it lies deep to muscle and its overlying fascia.

REFERENCES - CHAPTER III

1. Webber JC and Lamb DR: Statistics and research in physical education. The CV Mosby Co., St Louis, 1970.
2. Wagman IH and Lesse H: Maximum conduction velocities of motor fibers of ulnar nerve in human subjects of various ages and sizes. *J Neurophysiol* 14-15:235-244, 1951-52.
3. LaFratla CW and Smith OH: A Study of the relationship of motor nerve conduction velocity in the adult to age, sex and handedness. *Arch Phys Med* 43:407-412, 1964.
4. Mayer J: *Overweight: Causes, Costs and Controls*. Prentice-Hall Inc., Englewood Cliffs, New Jersey, 1968.
5. Larson LA, ed: *International Committee for Standardization of Physical Fitness Tests*. MacMillan Publishing Co. Inc., New York, 1974.
6. Snodgrass JG: *The Number Game. Statistics for Psychology*. The Williams and Wilkins Company. Baltimore, 1977.
7. Bannister R: *Brain's Clinical Neurology* 3rd ed. Oxford University Press. London, 1969.
8. Wadsworth H and Chanmuga A: *Electrophysical Agents in Physiotherapy. Therapeutic and Diagnostic Use*. Science Press. Marrichville NSW Australia, 1980.
9. Nelson RM: Effects of elbow position on motor conduction velocity of the ulnar nerve. *Phy Ther* 60:780-783, 1980.
10. Reid DC and Cummings GE: Factors in selecting the dosage of ultrasound. *Physio Canada* 25:5-0. 1973.
11. Smorko MP and Basmajian JV: *Clinical value of nerve conduction tests in electrodiagnosis*. Harper and Row Publishers. New York, 1977.
12. Scott B: Shortwave Diathermy. Chapter 7 from *Therapeutic Heat and Cold*. Volume Ten of *Physical Medicine*. Litch S, ed. Waverly Press, Inc., Baltimore, 1965.

D. CHAPTER IV - THE RESULTS

Eighteen healthy, informed volunteers (four males and 14 females) reporting no history of peripheral vascular disease, other disease, injury or medication known to cause neuropathies were examined. The age range was from 22 to 34 years (mean age 27.8 years). Only the dominant arm of each subject was tested. None of the subjects reported discomfort attributable to either the electrical stimulation technique or to the subcutaneous tissue temperature probe. Reliability tests for the measurement of the subcutaneous skinfold thickness; the measurement of the conduction velocity; and, the accuracy of electrode placement (as outlined in the appendix C) were completed by the author prior to data acquisition. The reliability and percent error tests indicated the author had a high reliability in performing the three above mentioned techniques (Table 4). The following statistical procedures were used in the analysis of the raw data:

The correlation between the one and zero minute pre-treatment subcutaneous tissue temperature was 0.9976, and the correlation between the zero and one minute post-treatment temperatures was 0.9975. The correlation between the one and the zero minute pre-treatment motor nerve conduction velocities was 0.8357, and the correlation between the zero and one minute post-treatment motor nerve conduction velocities was 0.8962 (Table 5). All correlation coefficients were statistically significant ($p < 0.01$).

The mean and standard deviation for the zero minute pre-treatment and the zero minutes post-treatment subcutaneous tissue temperature and motor nerve conduction velocities, for each modality, are given in Table 6. Table 7 illustrates the change (zero minute pre-treatment minus zero minute post-treatment) in subcutaneous tissue temperature and motor nerve conduction velocities associated with shortwave diathermy, ultrasound, and hot packs.

TABLE 4
Percent Error Tests for Measurement of Skinfold Thickness Layer,
Measurement of Conduction Velocity, and
Placement of Electrode

TEST PROCEDURE	PERCENT ERROR
Skinfold Thickness Layer	1.61%
Conduction Velocity	2.34%
Placement of Electrode	2.14%

TABLE 5
Correlation Coefficients for One and Zero Minute Pre-Treatment,
and Zero and One Minute Post-Treatment on
Subcutaneous Tissue Temperature and Motor Nerve Conduction Velocity

CRITERION MEASURE	ONE AND ZERO MINUTE PRE-TREATMENT	ZERO AND ONE MINUTE POST-TREATMENT
Subcutaneous Tissue Temperature	0.9976	0.9775
Motor Nerve Conduction Velocity	0.8357	0.8962

All values were statistically significant ($p < 0.01$).

TABLE 6
Mean and Standard Deviation of Zero Minute
Pre- and Zero Minute Post-Treatment Subcutaneous
Tissue Temperatures and Motor Nerve Conduction Velocities
For Shortwave Diathermy, Ultrasound, and Hot Packs

Modality	Subcutaneous Tissue Temperature (°C)		Motor Nerve Conduction Velocity (m/s)	
	Zero Minute Pre-Treatment	Zero Minute Post-Treatment	Zero Minute Pre-Treatment	Zero Minute Post Treatment
Shortwave Diathermy	35.4 (1.2)	38.4 (1.4)	62.47 (4.50)	67.31 (5.48)
Ultrasound	35.4 (2.1)	35.1 (2.1)	64.12 (4.15)	63.52 (3.81)
Hot Packs	35.6 (2.4)	38.7 (2.0)	62.14 (4.82)	68.42 (7.13)

(Standard Deviation)

TABLE 7
Change in Subcutaneous Tissue Temperature
and Motor Nerve Conduction Velocity Following The
Application of Shortwave Diathermy, Ultrasound, and Hot Packs

Modality	Change In Temperature (°C)	Change In Motor Nerve Conduction (m/s)
Shortwave Diathermy	+2.9	+4.83
Ultrasound	-0.4	-0.60
Hot Packs	+3.0	+6.28

" + " denotes increase " - " denotes decrease

The analysis of variance tests demonstrated statistically significant time main effects and interaction effects for both dependent variables ($p < 0.001$). The treatment effect was statistically significant for temperature ($p < 0.001$), but was not statistically significant for motor nerve conduction velocity ($p < 0.05$). Tables 8 and 9 demonstrate the probability values obtained in the analysis of variance for both subcutaneous tissue temperature and motor nerve conduction velocity.

TABLE 8

Analysis of Variance for Subcutaneous Tissue Temperature

Source of Variation	Sum of Squares	Degree of Freedom	Mean Squares	F Ratio
Treatment Main Effects	77.906	2	38.953	8.642*
Treatment x Subjects Within Groups	153.250	34	4.507	
Time Main Effects	92.250	1	92.250	151.157*
Time x Subjects Within Groups	10.375	17	0.610	
Treatment x Time Interaction	65.953	2	32.977	34.499*
Treatment x Time x Subjects Within Groups	32.500	34	0.956	
Subjects Within Groups	168.938	17	9.938	

* Statistically significant at the $p < 0.001$ level

TABLE 9

Analysis of Variance for Motor Nerve Conduction Velocity

Source of Variation	Sum of Squares	Degrees of Freedom	Mean Squares	F Ratio
Treatment Main Effects	41.273	2	20.637	0.845
Treatment x Subjects Within Groups	830.063	34	24.414	
Time Main Effects	331.664	1	331.664	25.136*
Time x Subjects Within Groups	224.313	17	13.195	
Treatment x Time Interaction	236.742	2	118.371	9.968*
Treatment x Time x Subjects Within Groups	403.750	34	11.875	
Subjects Groups	1193.125	17	70.184	

* Statistically significant at the $p < 0.001$ level

The Newman-Keuls post hoc tests (Tables 10 and 11) demonstrated that there was no statistically significant difference between the pre-treatment means for the shortwave diathermy, ultrasound and hot pack groups for both subcutaneous tissue temperature and motor nerve conduction velocity. Post-treatment, there was a statistically significant

difference between the ultrasound mean and the means observed for both shortwave diathermy, and hot packs for subcutaneous tissue temperature ($p < 0.01$). In comparing the post-treatment means of ultrasound, shortwave diathermy, and hot packs for motor nerve conduction velocity, there was a statistically significant difference between the ultrasound mean and the mean of shortwave diathermy at the $p < 0.05$ level and a statistically significant difference between the ultrasound mean and the hot pack mean at the $p < 0.01$ level. No statistically significant difference was observed between the post-treatment shortwave diathermy mean and that of the hot pack group for either subcutaneous tissue temperature or motor nerve conduction velocity.

A statistically significant difference between the pre- and post-treatment means was observed for shortwave diathermy and for hot pack on both subcutaneous tissue temperature and motor nerve conduction velocity ($p < 0.01$). However, no statistically significant difference between the pre-treatment and post-treatment means for ultrasound for either of the dependent variables was observed.

In comparing the remaining combinations between pre- and post-treatment differences in means for motor nerve conduction velocity, the following were found to be statistically significant ($p < 0.05$): a) pre-treatment shortwave diathermy and post-treatment hot pack, b) pre-treatment ultrasound and post-treatment hot pack, c) pre-treatment hot pack and post-treatment shortwave diathermy. For subcutaneous tissue temperature, there was a statistically significant difference ($p < 0.05$) between the following: a) pre-treatment shortwave diathermy and post-treatment hot pack, b) pre-treatment ultrasound and both post-treatment shortwave diathermy and hot pack, c) pre-treatment hot pack and post-treatment shortwave.

The Pearson Product Correlation matrices for each separate modality indicated no statistically significant correlation between any combination of the three dependent variables (skinfold thickness, change in subcutaneous tissue temperature, and change in motor nerve conduction velocity), except that observed between the change in motor nerve conduction velocity and the change in subcutaneous tissue temperature associated with hot packs (Table 12).

TABLE 10
Newman-Keuls Test Probability Summary for
Subcutaneous Tissue Temperature
(c°)

	Post 0 US (35.10)	Pre 0 US (35.4)	Pre 0 SWD (35.44)	Pre 0 HP (35.62)	Post 0 SWD (38.32)	Post 0 HP (38.65)
+++ Post 0 US (35.10)	-	NS*	NS	NS	0.01**	0.01
Pre 0 US (35.4)	-	-	NS	NS	0.01	0.01
Pre 0 SWD (35.44)	-	-	-	NS	0.01	0.01
Pre 0 HP (35.62)	-	-	-	-	0.01	0.01
Post 0 SWD (38.32)	-	-	-	-	NS	NS
Post 0 HP (38.65)	-	-	-	-	-	-

*NS = statistically non-significant

** 0.01 = statistically significant at the $p \leq 0.01$ level

+++ For both Tables 10 and 11:

Post 0 US = 0 minute post-treatment ultrasound

Pre 0 US = 0 minute pre-treatment ultrasound

Pre 0 SWD = 0 minute pre-treatment shortwave diathermy

Pre 0 HP = 0 minute pre-treatment hot pack

Post 0 SWD = 0 minute post-treatment shortwave diathermy

Post 0 HP = 0 minute post-treatment hot pack

TABLE 11
Newman-Keuls Test Probability for
Motor Nerve Conduction Velocity (m/s)

	Pre 0 HP (62.14)	Post 0 US (62.47)	Pre 0 SWD (63.52)	Pre 0 US (67.31)	Post 0 SWD (67.31)	Post 0 HP (68.42)
+++ Pre 0 HP (62.14)	-	NS*	NS	0.01**	0.01	0.01
Pre 0 SWD (62.47)	-	-	NS	NS	0.01	0.01
Post 0 US (63.52)	-	-	-	NS	0.05	0.01
Pre 0 US (64.12)	-	-	-	-	NS	0.01
Post 0 SWD (67.31)	-	-	-	-	-	NS
Post 0 HP (68.42)	-	-	-	-	-	-

*NS = statistically non-significant

** 0.01 = statistically significant at the $p \leq 0.01$ level

+++ See Table 10

TABLE 12
Correlation Matrices for Change in
Subcutaneous Tissue Temperature, Change in
Motor Nerve Conduction Velocity, and
Skinfold Thickness for Each Modality

		Skinfold Thickness	Change In Tissue Temperature	Change In Motor Nerve Conduction
1.Shortwave Diathermy				
	Skinfold Thickness	1.00	-	
	Tissue Temperature	-0.1597	1.000	
	Motor Nerve Conduction	-0.2861	0.0709	1.000
2.Ultrasound				
	Skinfold Thickness	1.00	-	
	Tissue Temperature	0.0545	1.000	
	Motor Nerve Conduction	-0.2939	0.2888	1.000
3.Hot Pack				
	Skinfold Thickness	1.00	-	
	Tissue Temperature	0.412	1.000	
	Motor Nerve Conduction	0.2206	0.7256*	1.000
N=18		DF=16	(r @ 0.05=0.4863)	(r @ 0.01=0.5897)

* Statistically significant at the 0.01 level.

E. CHAPTER V - DISCUSSION

Both subcutaneous tissue temperature and motor nerve conduction velocity increased significantly, and similarly, following the administration of shortwave diathermy and hot packs. For this reason, the increased conduction velocity is attributed to the heating effects of both modalities on motor nerves. These findings are in agreement with previous studies having used similar modalities and reporting an increase in motor nerve conduction velocity associated with an increase in subcutaneous tissue temperature.¹⁻³

Ultrasound was observed to produce a small and a statistically non-significant decrease in both subcutaneous tissue temperature and motor nerve conduction velocity. This result is in general agreement with studies reported by Zankel², Farmer⁴, and Madsen and Gersten⁵. These authors concluded that continuous ultrasound given at approximately one watt per square centimeter for five to ten minutes produced a decrease in motor nerve conduction velocity of the ulnar nerve²⁻⁵. However, the authors disagreed to why this decrease occurred. Zankel² did not find a significant change in surface skin temperature, but did observe a statistically significant decrease in motor nerve conduction velocity after ten minutes of ultrasound over the ulnar nerve pathway in the forearm between the elbow and the wrist. Since he observed that ultrasound and cold packs both produced a decrease in ulnar motor nerve conduction velocity, the reduction in velocity was attributed to some factor other than the thermal effects of ultrasound. Zankel² suggested a micromassage action of the ultrasound might produce a change in the rate of exchange of transmembranal electrolytes, resulting in a decrease in motor nerve conduction velocity.

Farmer⁴ did not measure temperature during testing but he did conclude that the mechanical effects of ultrasound overpowered the thermal effects at intensities of one, 1.5, and two watts per square centimeter. He postulated that it was the mechanical effects of ultrasound which produced a decrease in motor nerve conduction velocity. Farmer⁴ suggested that the biphasic response of ultrasound enables clinicians to select dosages appropriate to their treatment objectives; i.e., dosages of 0.5 and 2.5 watts per square centimeter increased motor nerve conduction velocity while dosages of 1.0, 1.5 and 2.0 watts per square centimeter decreased motor nerve conduction velocity.

Madsen and Gersten⁵ reported that intensities of 0.88 and 1.28 watts per square centimeter produced a decrease in ulnar motor nerve conduction velocity. This decrease in motor nerve conduction velocity was associated with a slight, but statistically non-significant, decrease in tissue temperature. The mechanism for this reduction was not discussed.

None of the previously reported studies discussed the possible cooling effects of the coupling medium used. It has been reported that Aquasonic gel[®] has a definite cooling effect on tissue temperature^{6, 7, 11}. However, to what depth the cooling effect will take place was not discussed. This cooling effect was found consistently with each subject in the present experiment. In most subjects, application of the Aquasonic gel[®] resulted in an immediate decrease in the subcutaneous tissue temperature. Figure 8 illustrates the change in subcutaneous tissue temperature immediately prior to the application of the Aquasonic gel[®], during the five minute ultrasound treatment, and immediately following the treatment. In the majority of the subjects, the post-treatment subcutaneous tissue temperature did not return to the original temperature that existed before the application of the Aquasonic gel[®]. The net overall loss in the subcutaneous tissue temperature was 0.2 degrees Celsius. It would appear that the heating effects of ultrasound at one watt per square centimeter for five minutes was not sufficient to counteract the cooling effect of the Aquasonic gel[®].

It is suggested that the decrease in ulnar motor nerve conduction velocity associated with sonation might be attributable to the cooling effects of Aquasonic gel[®]. However, as both subcutaneous tissue temperature and motor nerve conduction velocity changes were statistically non-significant, this suggestion must be made with caution and requires further study to be substantiated.

Kramer¹¹, in his study on the mechanical and thermal effects of ultrasound, also found a cooling effect of the Aquasonic gel[®]. In his study, Kramer found a rapid fall of 2.6 degrees Celsius in subcutaneous tissue temperature during the first five minutes of pulsed and placebo ultrasound. This decrease in subcutaneous tissue temperature was associated with a decrease in motor nerve conduction velocity. Kramer attributed the decrease in motor nerve conduction velocity to the cooling effect of the Aquasonic gel[®] and not to the mechanical effects of ultrasound.

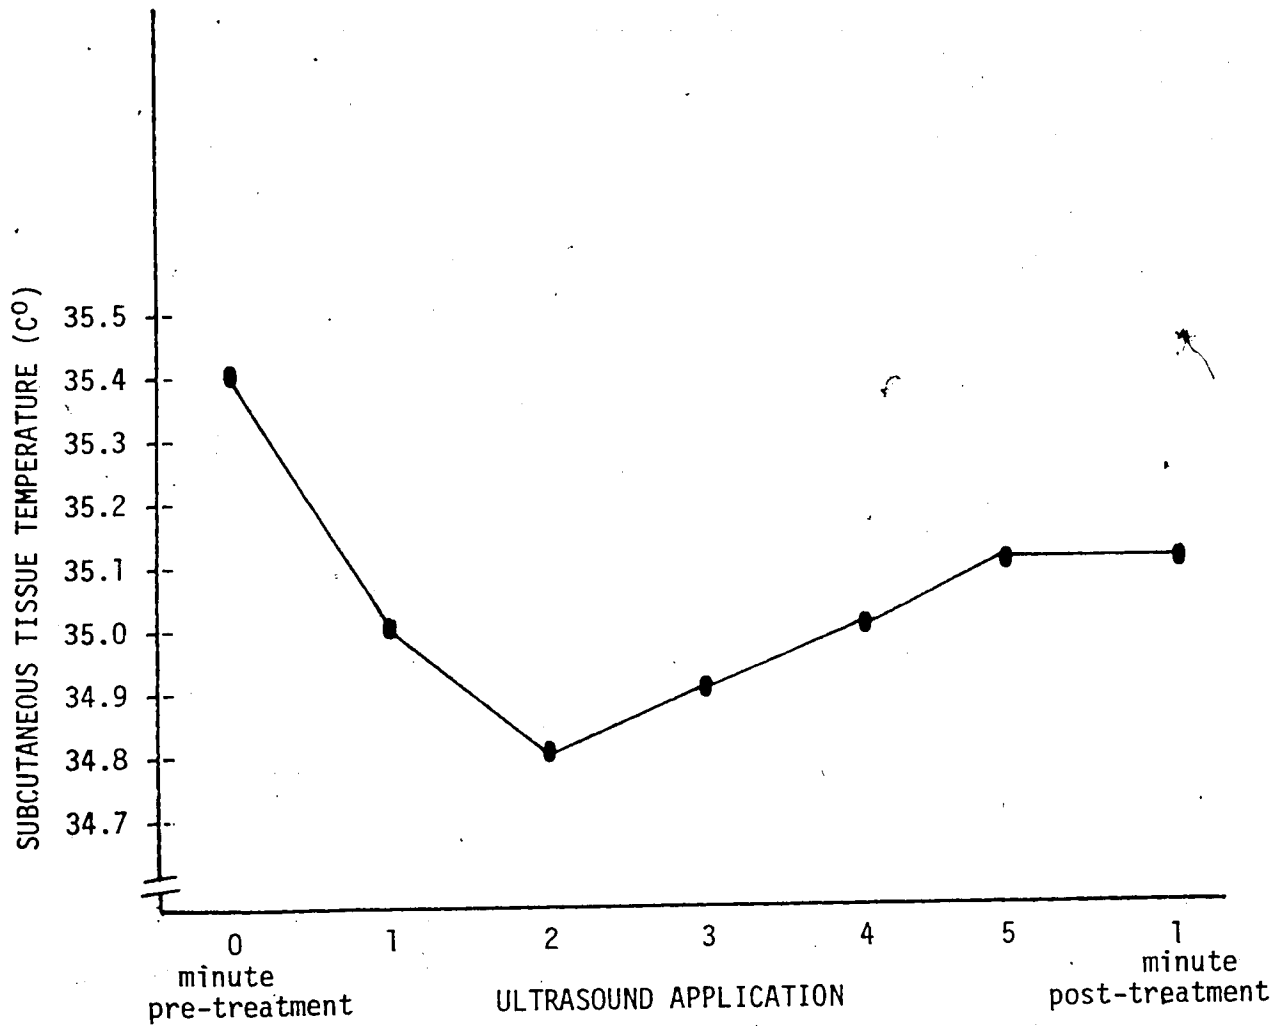


Figure 8

Change in Subcutaneous Tissue Temperature
During the Application of Ultrasound

important factor in absorbing heat produced by the shortwave diathermy and ultrasound.

TABLE 13

Comparison of Mayer's Standard of Minimum Triceps Skinfold Thickness
Indicating Obesity and Triceps Skinfold Thickness
Of Subjects (millimeters)

AGE (YEARS)	MAYER'S STANDARD FOR MALES	MALE SUBJECTS	MAYER'S STANDARD FOR FEMALES	FEMALE SUBJECTS
22	18	7.12*	28	26.1*
23	18	-	28	26.9*
24	19	-	28	15.74*
25	20	5.79*	29	14.1*
26	20	-	29	20.1*
27	21	-	29	22.9*
28	22	-	29	
29	22	-	29	17.1*
30-50	23	13.49**	30	17.7***

- no subjects in that age group
 * one subject in that age group
 ** mean of two subjects in that age group
 *** mean of six subjects in that age group

Adapted from: Mayer J: Overweight: Causes, Costs and Control.
 Prentice-Hall, Inc. Englewood Cliffs, New Jersey, 1968.

Secondly, the selective heating effects of shortwave diathermy on the subcutaneous needle probe may have affected the relationship between the change in subcutaneous tissue temperature and the change in motor nerve conduction velocity. Thirdly, in the case of ultrasound, the cooling effect of the Aquasonic gel[®] may have counteracted the heating effect of ultrasound and therefore masked the relationship between change in subcutaneous tissue temperature and change in motor nerve conduction velocity.

From the results of the statistical analysis of the data of this study, it is impossible to draw any firm conclusions about the relationship between the change in subcutaneous tissue temperature, the change in motor nerve conduction velocity, and the skinfold thickness layer. It does not seem likely that the subcutaneous tissue layer is an important factor in the subcutaneous tissue temperature nor the change in motor nerve conduction velocity.

Woodbury¹⁴ stated that both the physical properties and fiber geometry help to determine the conduction speed of nerves. He stated the most important factor is the extent of the depolarization induced by an increase in sodium permeability. The greater the sodium permeability is, the greater the sodium influx will be resulting in an increase in the rate of rise of the action potential. This increase in the rate of rise of the sodium input current will increase the flow of the local circuit currents and results in a quicker excitation of adjacent regions of the nerve fiber and, thus, increase nerve conduction velocity.

A reduction in the degree of depolarization of the nerve fiber to reach the threshold of the action potential also increases nerve conduction velocity. A reduction in threshold means that less sodium input current is needed for depolarization and, therefore, there is less movement of sodium ions resulting in an increase in nerve conduction velocity¹⁴.

A smaller capacity of charge on the nerve fiber membrane decreases nerve conduction velocity. This smaller capacity of charge on the nerve fiber decreases the length of time the local circuit currents must flow to depolarize the nerve fiber membrane¹⁴. Increase in the concentration of mobile ions in both the interstitial fluid and intracellular plasma results in an increase in nerve conduction velocity. This increase in concentration increases the local circuit flow of sodium influx and potassium efflux and,

therefore, increases nerve conduction velocity.

Furthermore, in myelinated fibers, conduction velocity is dependent on the thickness of the myelin sheath relative to the axon diameter and on the distance between nodes. Conduction speed has a linear relationship with the diameter of the myelinated fiber¹⁴.

From the review of the literature and from what Woodbury's comments on the effect of heat on nerve conduction, the author would like to propose the following possibilities as answers to the question of how heat causes an increase in nerve conduction in the studies described in this thesis. It seems possible that the increase in heat caused by shortwave diathermy and hot packs could have resulted in an increase in the sodium permeability of the nerve fibers within the ulnar nerve and/or an increase in the flow of the local circuit currents, and/or a decrease in the resting membrane potential. Other possibilities are: an increase in temperature might have resulted in an increase in the agitation of the sodium and potassium ions around the nerve membrane and thus promote the influx and efflux of sodium and potassium through the membrane. A decrease in the viscosity of the nerve fiber cytoplasm would also facilitate the ionic current flow.

As stated previously, the author believes that the decrease in subcutaneous tissue temperature and motor nerve conduction velocity associated with ultrasound was caused by the cooling effect of the Aquasonic gel[®]. The cooling effects of the Aquasonic gel[®] may have produced a slowing of the efflux of potassium which would then delay the recovery of the nerve fiber back to its resting state.

In summary, it seems that the increase in temperature brought about by shortwave diathermy and hot packs might have had an effect on each part of the sequences that makes up an action potential. The decrease in temperature brought about by the cooling effect of the Aquasonic gel[®] used with the application of ultrasound might have had an effect on the mechanism of recovery of the nerve fiber back to its resting state.

REFERENCES - CHAPTER V

1. Currier DP and Nelson RM: Changes in motor nerve conduction velocity induced by exercise and diathermy. *Phy Ther* 49:146-152, 1969.
2. Zankel HT: Effect of physical agents on motor nerve conduction velocity of the ulnar nerve. *Arch Phys Med* 47:787-792, 1966.
3. Abramson PD, Chu LSW, Tuck S Jr, Lee SW, Richardson G, Levin M: Effect of tissue temperature and blood flow on motor nerve conduction. *JAMA* 198:1082-1088, 1966.
4. Farmer WC: Effect of intensity of ultrasound on conduction of motor axons. *Phy Ther* 48:1233-1237, 1968.
5. Madsen PW, Gusten JW: The effects of ultrasound on conduction velocity of peripheral nerve. *Arch Phys Med Rehabil* 42:645-649, 1961.
6. Griffin JE: Physiological effects of ultrasound energy as it is used clinically. *Phy Ther* 46:18-26, 1966.
7. Reid DC, and Cummings, GE: Factors in selecting the dosage of ultrasound. *Phsio Canada* 25:5-9, 1973.
8. Scott BO: The effects of metal on shortwave diathermy field distribution. *Ann Phys Med* 7:238-244, 1953.
9. Lehmann JT, ed: *Therapeutic Heat and Cold*. Williams and Wilkins. Baltimore, 1982.
10. Licht S., ed: *Therapeutic Heat and Cold*. Volume Two of *Physical Medicine*. Waverly Press Inc., Baltimore, 1965.
11. Wadsworth H, and Chanmugan A: *Electrophysical agents in physiotherapy: Therapeutic and diagnostic use*. Science Press Manichville NSW Australia, 1980.
12. Lehmann JT, Silverman DR, Baum BA, Kirk NL, Johnston VC: Temperature distribution in the human thigh produced by infrared, hot pack, and microwave applications. *Arch Phys Med Rehabil* 47:291-299, 1966.
13. Kramer JF: Evaluation of the mechanical and thermal effects of ultrasound. (In print). *Arch Phys Med Rehabil*, 1984.
14. Ruch TC, Patton HD: *Physiology and Biophysics*. W.B. Saunders Co. Philadelphia, 1965.

F. CHAPTER VI - CONCLUSION

The purpose of this study was to examine the effects of shortwave diathermy, ultrasound and hot packs to the subcutaneous tissue temperature and the motor nerve conduction velocity of the ulnar nerve. A sample of 18 informed adults was used, only the dominant arm of each subject was tested. Each subject was tested three different times, once for each modality.

The testing procedure involved taking two pre-treatment tests of subcutaneous tissue temperature and motor nerve conduction velocity, applying the modality appropriate for that particular session and, at the end of the treatment, two more tests on subcutaneous tissue temperature and motor nerve conduction velocity. On their first visit to the experimental laboratory, a skinfold thickness measurement of the triceps and the forearm was taken on each subject.

The data was analyzed by a two by three analysis of variance with repeated measurement. A Newman-Keuls tests was performed to analyze the differences between the cell means. A Pearson Product Correlation Coefficient was performed to investigate whether there was a correlation between the change in the subcutaneous tissue temperature, and the change in motor nerve conduction velocity and the skinfold thickness layer for each modality.

Results indicated that shortwave diathermy and hot packs produced a statistically significant increase in both subcutaneous tissue temperature and motor nerve conduction velocity, whereas ultrasound did not significantly change subcutaneous tissue temperature nor motor nerve conduction velocity. The Pearson Product Correlation Coefficient demonstrated a statistically significant correlation between the change in subcutaneous tissue temperature and the change in motor nerve conduction velocity with hot packs only. There was no significant correlation between the skinfold thickness layer or the change in subcutaneous tissue temperature or the change in motor nerve conduction velocity for any of the three modalities.

Therefore, in conclusion, within the restrictions of this study, it may be stated that shortwave diathermy and hot packs produce a statistically significant increase in subcutaneous tissue temperature and motor nerve conduction velocity of the ulnar nerve, whereas ultrasound does not. The increase in motor nerve conduction velocity of the

ulnar nerve is attributable to the heating effect caused by shortwave diathermy and hot packs.

G. BIBLIOGRAPHY

- Abbott R: The positive and negative heat production associated with nerve impulse. Proc Roy Soc. Series B 148:149-187, 1958.
- Abramson DI, Bell Y, Ryal H. Changes in blood flow, oxygen uptake and tissue temperature produced by therapeutic agents: II. Effects of shortwave diathermy. Am J Phys Med 39:87-95, 1960.
- Abramson DI, Burnett S, Bell Y, Tuck S, Rejal H, Fleischer CJ. Changes in blood flow, oxygen uptake and tissue temperature produced by therapeutic physical agents: I. Effect of ultrasound. Am J Phys Med 39:51-62, 1960.
- Abramson DI, Chu LSW, Tuck S, Lee SW, Richardson G, Levin M. Effect of tissue temperature and blood flow on motor nerve conduction. JAMA 198:1082-1088, 1966.
- Adrian ED: The Recovery Process of Excitable Tissue. Part II. J Physiol 50:193-225, 1921.
- Bannister R. Brain's Clinical Neurology. 3rd ed. Lond Toronto: Oxford University Press, 1969.
- Brobeck JR ed.: Best and Taylor's Physiological Basis of Medical Practice. Ninth edition. The Williams and Wilkins Co. Baltimore, 1973.
- Brunner GD, Lehmann JA, McMillan KE, Lane K, Bell JW. Can ultrasound be used in the presence of surgical metal implants: An experimental approach. Phys Ther Review 38:823-824, 1958.
- Coakley WT. Biophysical effects of ultrasound at therapeutic intensities. Physiotherapy 64:166-169, 1978.
- Checkler, NW, Rüssakov AD, Prevo DI. Ulnar nerve conduction velocity: Effect of elbow position on measurement. Arch Phys Med Rehabil 52:362-365, 1971.
- DeJesus PV, Hausmanova-Petrusewicz I, Barchi RL: The effect of cold on nerve conduction of slow and fast nerve fibers. Neurol 23:1182-1189, 1973.
- Delbeke J, Kopec J, McComas AJ: Effects of age, temperature and disease on the refractoriness of human nerve and muscle. J Neurol Neurosurg Psychiat 41:65-71, 1978.
- Dotz E: Differential thermosensitivity of mammalian A fibers. Acta Physiol Scand

- 29:91-108, 1954.
- Douglas WW and Malcolm JL: The Effect of Localized Cooling on Conduction in Cat Nerves. *J Physiol* 130:53-71, 1955.
- Dyson M, Pond JB. The effects of ultrasound on circulation. *Physiotherapy* 59:284-287, 1973.
- Echandi ELR and Prezzi RS: Effect of Low Temperature on the Sciatic Nerve. *J Cell Biol* 33:491-498, 1968.
- Esmat N. Investigations on the effects of different doses of ultrasonic waves on the human nerve conduction velocity. *J Egypt Med Assoc* 58:395-402, 1975.
- Faris P. Ultrasound: The dosage question. *Physio Canada* 21:155-158, 1969.
- Farmer WC. Effect of intensity of ultrasound on conduction of motor axons. *Phys Ther* 48:1233-1237, 1968.
- Ferguson GA. *Statistical Analysis in Psychology and Education*. Toronto: McGraw-Hill Book Co., 5th ed., 1981.
- Frankenhaeuser B, Moore LE: The effect of temperature on the sodium and potassium permeability changes in myelinated nerve fibres of *Xenopus laevis*. *J Physiol (Lond)* 169:431, 1963.
- Gasser HS. Nerve activity as modified by temperature changes. *Am J Physiol* 97:254-270, 1931.
- Gasser HS: The classification of nerve fibers. *Ohio J Sci* 41:145-159, 1941.
- Glass GV, Stanley JC. *Statistical Methods in Education and Psychology*. Prentice Hall. Englewood Cliffs, NJ, 1970.
- Griffen JE. Physiological effects of ultrasound energy as it is used clinically. *J Am Phys Ther* 46:18-26, 1966.
- Halar EM, DeLisa JA, Brozovich, FC. Peroneal nerve conduction velocity: The importance of temperature correction. *Arch Phys Med Rehabil* 62:439-443, 1981.
- Halar EM, DeLisa JA, Brozovich FV. Nerve conduction velocity: Relationship of skin, subcutaneous and intramuscular temperature. *Arch Phys Med Rehabil* 61:199-203, 1980.
- Hall JS, Scoville CR, Greathouse DS. Ultrasound's effect on conduction latency of the superficial radial nerve in man. *Phys Ther* 61:345-350, 1981.

- Herrick, JF. Temperatures produced in tissues by ultrasound: Experimental study using various techniques. *Jr Acc Soci Am* 25:12-16, 1953.
- Hill TS: Heat Production in Nerve and Muscle. *Ann Rev Physiol* 21:1-18, 1959.
- Hodgkin AL and Katz B: The Effect of Temperature on the Electrical Activity of the Giant Axon of the Squid. *J Physiol* 109:240-249, 1949.
- Hodgkin AL, Huxley AF, and Katz B: Measurement of Current Voltage Relations in the Membrane of the Giant Axon of the Loligo. *J Physiol* 116:424-448, 1952.
- Hovind H, Nielsen SL. Local blood flow after shortwave diathermy: Preliminary report. *Arch Phys Med* 55:217-221, 1974.
- Huxley JB. Conduction velocity and diameter of nerve fibers. *Amer J Physiol* 127:131-134, 1939.
- Janis P. Ultrasound: The dosage question. *Physio Canada* 21:155-159, 1969.
- Katz B: Nerve Muscle and Synapse. McGraw Hill Book Co. Toronto, 1966.
- Keele CA and Neil E, eds.: Samson Wright's Applied Physiology. Eleventh Edition. Oxford University Press. Toronto, 1965.
- LaFratta CW, Canestrai RE. A comparison of sensory and motor nerve conduction velocities as related to age. *Arch Phys Med Rehabil* 47:286-290, 1966.
- LaFratta CW, Smith OH. A study of the relationship of motor nerve conduction velocity in the adult to age, sex and handedness. *Arch Phys Med Rehabil* 45:407-412, 1964.
- Larson, LA, ed. International Committee for Standardization of Physical Fitness Tests. New York: MacMillan Publishing Co., 1974.
- Lehmann JT, ed. Therapeutic Heat and Cold. Baltimore: Williams and Wilkins, 1982.
- Lehmann JT, DeLateur BJ, Silverman DH. Selective heating effects of ultrasound in human beings. *Arch Phys Med Rehabil* 47:331-339, 1966.
- Lehmann JT, DeLateur BJ, Stonebridge JB. Selective muscle heating by shortwave diathermy with a helical coil. *Arch Phys Med Rehabil* 50:117-123, 1969.
- Lehmann JT, DeLateur BJ, Warren CG, Stonebridge JS. Heating produced by ultrasound in bone and soft tissue. *Arch Phys Med Rehabil* 48:397-401, 1967.
- Lehmann JT, DeLateur BJ, Warren CG, Stonebridge JB. Heating of joint structures by ultrasound. *Arch Phys Med Rehabil* 49:28-30, 1968.
- Lehmann JT, DeLateur BJ, Warren CG, Stonebridge JB. Therapeutic temperature

- distribution produced by ultrasound as modified by dosage and volume of tissue exposed. Arch Phys Med Rehabil 48:662-668, 1967.
- Lehmann JT, Guy AW, DeLatuer BJ, Stonebridge JB, Warren CG. Heating patterns produced by shortwave diathermy using helical induction coil application. Arch Phys Med Rehabil 49:193-198, 1968.
- Lehmann JT, Silverman DR, Baum BA, Kirk ML, Johnston VC. Temperature distribution in the human thigh produced by infrared hot pack and microwave application. Arch Phys Med Rehabil 47:291-299, 1966.
- Lehmann JT, Stonebridge JB, DeLatuer BJ, Warren CG, Halar EH. Temperatures in human thighs after hot pack treatment followed by ultrasound. Arch Phys Med Rehabil 59:472-475, 1978.
- Lenman JAR, Ritchie AE. Clinical Electromyography. 2nd ed. New York: JB Lippincott, 1977.
- Liberson WT, Gratzner M, Zalis A, Grabinski B. Comparison of conduction velocities of motor and sensory fibers determined by different methods. Arch Phys Med Rehabil 47:17-23, 1966.
- Licht S, ed. Therapeutic Heat and Cold. Volume Two of Physical Medicine. Baltimore: Waverly Press, 1965.
- Lucas K: The temperature coefficient of the rate of conduction in nerve. J Physiol 37:117-121, 1908.
- Lundberg A: Potassium and the differential thermosensitivity of membrane potential: Spike and negative after potential in mammalian A and C fibers. Acta Physiol Scand 15(20), 1948.
- Madsen PW, Gusten JW. The effects of ultrasound on conduction velocity of peripheral nerve. Arch Phys Med Rehabil 42:645-659, 1961.
- Mayer J. Overweight: Causes, costs and control. Engelwood Cliffs, NJ: Prentice Hall, Inc., 1968.
- Mortimer A, Lee N. An International Symposium on Therapeutic Ultrasound. Proceedings CPA, Winnipeg, 1981.
- Nelson RM. Effects of elbow position on motor conduction velocity of the ulnar nerve. Phys Ther 60:780-783, 1980.

- Oakley EM. Application of continuous beam ultrasound at therapeutic levels. *Physiotherapy* 64:169-172, 1978.
- Paintal AS: Block of conduction in mammalian myelinated nerve fibers by low temperatures. *J Physiol* 180:1-19, 1965.
- Paintal AS: Effects of temperature on conduction in single vagal and saphenous myelinated nerve fiber of the cat. *J Physiol* 180:20-49, 1965.
- Reid DC, Cummings GE. Factors in selecting the dosage of ultrasound. *Physio Canada* 25:5-10, 1973.
- Ruch TC, Patton HD: *Physiology and Biophysics*. W.B. Saunders Co. Philadelphia, 1965.
- Schoepfle GM and Erlanger J: The action of temperature on the excitability spike height and configuration and the refractory period observed in the response of single modulated nerve fiber. *Amer J Physiol* 134:694-704, 1941.
- Smorto MP and Basmajian JV: *Clinical Electroneurography*. The Williams and Wilkins Co. Baltimore, 1979.
- Smorto MP, Basmajian JV. *Electrodiagnosis*. Harper Row Publishers, London, 1977.
- Snodgrass JG: *The Number Game: Statistics for Psychology*. The Williams and Wilkins Co., Baltimore, 1977.
- Tasaki I, Fujita M: Action currents of single nerve fiber as modified by temperature changes. *J Neurophysiol* 11:310-315, 1948.
- Tasaki I: The excitatory and recovery processes in the nerve fiber as modified by temperature and chemicals. *Acta Biochem Biophys* 3:498-509, 1949.
- Wadsworth H, Chanmuga A. *Electrophysican agents in diagnostic physiotherapy: Therapeutic and diagnostic use*. Science Press, Manichville NSW Australis, 1980.
- Wagman IH, Lesse H. Maximum conduction velocities of motor fibers of ulnar nerve in human subjects of various ages and sizes. *J Neurophysiol* 14-15:235-244, 1951-52.
- Webber JC, Lamb DR. *Statistics and research in physican education*. St. Louis: The CV Mosby Co., 1970.
- Zankel HT. Effect of physical agents on motor nerve conduction velocity of the ulnar nerve. *Arch Phys Med Rehabil* 47:787-792, 1966.

H. APPENDIX A - FORMS USED IN RESEARCH PROJECT

QUESTIONNAIRE FOR SCREENING POTENTIAL SUBJECTS

TO: Potential subjects who have agreed to participate in this study to examine the effects of shortwave diathermy, ultrasound, and hot packs on motor nerve conduction velocity.

FROM: Yvette D Claveau

In order that the results of this study be as valid as possible, please complete the details below. I assure you that confidentiality shall be strictly maintained.

PERSONAL DATA FORM

NAME: _____

ADDRESS: _____

PHONE NUMBER: _____

AGE: _____ YEARS _____ MONTH

WEIGHT: _____ kilograms
centimeters

HEIGHT: _____

TRICEPS SKINFOLD THICKNESS TEST: _____

FOREARM SKINFOLD THICKNESS TEST: _____

**PLEASE TURN PAGE AND COMPLETE THE SECOND PORTION OF THIS
QUESTIONNAIRE**

Please indicate by placing a check in the appropriate column whether you have had any of the following medical problems:

YES

NO

-Diabetes

-Metal implant

-Disease of the nervous system

-History of vascular disease

-History of damage to the ulnar nerve

-Previous injury of elbow (fracture, dislocation)

-Loss of sensation in the forearm and hand

-Lead Poisoning

DATE: _____ SIGNED: _____

INFORMED CONSENT FORM FOR EXPERIMENT

Effects of Shortwave diathermy, ultrasound, and hot pack on motor nerve conduction velocity.

I (*print name*) _____ do hereby agree to participate in this research study on the effects of shortwave diathermy, ultrasound, and hot pack on motor nerve conduction velocity. I have been given a full explanation of the procedure, the risks and the scientific benefit. I have been advised that I may withdraw from the experiment at any time I so choose.

DATE: _____ SUBJECT'S SIGNATURE: _____

I hereby certify that I have given to the above person an explanation of the experimental procedure, its risks and benefits.

PRINCIPAL INVESTIGATOR: _____

I hereby certify that I was a witness to the above explanation and signatures.

DATE: _____ WITNESS: _____

INFORMATION TO POTENTIAL SUBJECTS

Shortwave diathermy, ultrasound, and hot packs are commonly used modalities in physical therapy treatments. The purpose of this study is to compare the heating effect of these modalities on the conduction velocity of the ulnar nerve.

There will be three treatment sessions, each of approximately forty minutes. There must be at least 48 hours between each treatment session. Each treatment will be applied within the normal therapeutic procedures.

In the shortwave diathermy treatment, you will have a monode placed over your forearm near the elbow. During the treatment you are to feel a comforting warm heat.

In the ultrasound treatment, a coupling agent (gel) will be applied to your forearm. You will then receive a five minute treatment of ultrasound. The ultrasound head is moved over the treatment area in a slow, circular manner. You will feel warmth from the ultrasound.

In the hot pack group, you will have a hot pack covered in a terry cloth placed on your forearm for twenty minutes. You will feel a gentle warmth from the hot pack during this time.

If, during any of the three treatments, you feel the shortwave diathermy, ultrasound or hot pack is getting too warm, you are to tell the experimenter and the treatment will be stopped.

The following procedures will be carried out at each session:

On arrival at the laboratory, a skinfold thickness measurement will be taken of your forearm and arm. Your hand and arm will be cleansed with isopropyl alcohol. Electrodes will be taped on your hand and a ground electrode on a finger. Two points of stimulation will be marked on your arm. A needle probe will be inserted diagonally into the treatment area of your forearm. You are given five minutes rest for temperature stabilization.

Once your temperature is stabilized, the first pre-test motor nerve conduction velocity will be taken. This test will be repeated one minute later and the treatment to which you have been assigned for that particular visit administered in accordance with the above description. Following treatment, two more motor nerve conduction velocities will be taken at one minute intervals. All electrodes and the needle probe will then be removed, your forearm wiped clean and you may leave.

You are free to ask the investigator any questions. You are free to withdraw from the experiment any time you choose.

All identification and personal information will be kept strictly confidential.

Thank you for your support in this study.

I. APPENDIX B - CALIBRATION OF EQUIPMENT

Calibration of the Shortwave Diathermy Unit

The calibration of the output of the Siemens 708 shortwave diathermy unit was done in the following manner. This procedure was performed by a technical representative of Electromed Services. A calibration light test box from ENRAF NONIUS DELEFT Manufacturing Company was used. The monode was centered on the side of the light box labelled monde circuplode. The shortwave diathermy machine was turned on and the intensity was turned on as high as possible (i.e., 5 on the Siemens 708 model). Once the shortwave diathermy machine was in tune with the light box, the photo detector on the light box was read. As the photo detector reads out in direct current milliamperes this was then converted into watts by the use of the conversion table provided. The watts indicated by the conversion table were compared to the watts output indicated on the Siemens 708 and, if the two wattages were the same, the machine was considered calibrated. If not, adjustments were made to make the two wattages the same.

Calibration of the Ultrasound Unit

Calibration of the intensity of the Burdick UT 4300 Ultrasound Machine was carried out in the following manner by the experimenter with the use of the Russian Ultraschalleistungsmessgerat N MY-3 unit. The water container of the Russian N MY-3 unit was filled to the water mark with distilled water. The ultrasound head was covered on its outer circumference by foam padding so that the ultrasound head fitted snugly into the opening provided for the ultrasound head found on top of the water container. The ultrasound head was parallel to the water line mark. The watt indicator was set at six watts total output (equal to one watt per square centimeter). The ARR switch was pushed down so as to release the metal plate. The ultrasound machine was turned on to an intensity of one watt per square centimeter. If the intensity output of the ultrasound machine was accurate, the red indicator corresponded exactly with a vertical line on the upper surface of the watt indicator. If the intensity was not accurate, the red indicator was off the vertical line. Adjustment of the intensity output was then made on the ultrasound machine by turning the dial on the underside of the machine until the red indicator and the vertical line and the wattage output indicated on the ultrasound machine all

Calibration of the Hot Pack

The same hot pack was used throughout the experiment. The water temperature of the hydrocollator from which the hot pack was removed was tested prior to each use of the hot pack. Unless the water temperature was between 70 degrees Celsius, plus or minus five degrees Celsius, the hot pack was not used. To insure that no one else used the hot pack, a message was taped to the hydrocollator requesting all persons not to use that particular hot pack.

Calibration of the Needle Probe, Digital Thermometer and Scanning Thermometer

A Fisher Oven of 0.7 cubic feet and a Propper Chemical Thermometer (temperature range of 10 to 200 degrees Celsius) was used for the calibration of the two needle probes and the two thermometers. Calibration was done as follows. The needle probe was taped to the chemical thermometer so that the tip of the needle probe was close to, but not touching, the bulb of the chemical thermometer. The two were inserted into the middle hole of the Fisher oven and secured in place with tape (the two remaining holes on the oven were blocked with cork). The needle probe was connected to the digital thermometer and the oven was turned on. Once the Fisher oven had heated the chemical thermometer and needle probe to slightly above 43 degrees Celsius (the highest temperature the digital thermometer will record), the oven was turned off and the chemical thermometer and needle probe were allowed to cool. Once the digital thermometer recorded 43 degrees Celsius, the temperature on the chemical thermometer was recorded. Thereafter, as the temperature on the chemical thermometer decreased every .5 degrees Celsius, the corresponding temperature on the digital thermometer was recorded. This process continued until the chemical thermometer had reached 27.5 degrees Celsius, well below any temperature expected to occur during the experimental procedure. This same procedure was repeated with the scanning thermometer. The highest temperature that the scanning thermometer recorded is 50 degrees Celsius and, therefore, the oven was turned off once the temperature has reached 50 degrees Celsius. The procedure of temperature recording during the cooling of the chemical thermometer and needle probe was the same procedure as that used with the digital thermometer (see pages 73 to 76).

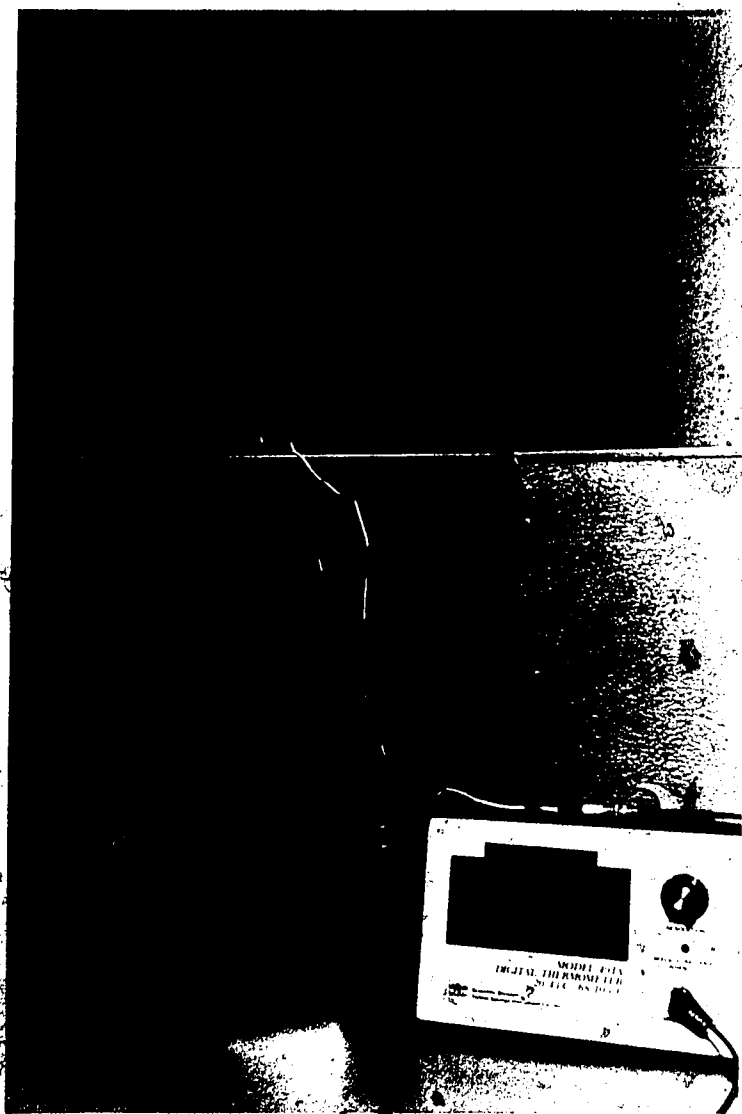


Figure 10

Calibration of a Needle Probe
With the Digital Thermometer

NEEDLE PROBE #1 -- DIGITAL THERMOMETER #1

Temperature - Chemical Thermometer	Temperature - Digital Thermometer
44.0	42.9
43.5	42.4
42.5	41.6
42.0	41.5
41.5	41.0
41.0	40.8
40.5	40.3
40.0	40.0
39.5	39.7
39.0	39.3
38.5	38.8
38.0	38.9
37.5	38.2
37.0	38.4
36.5	37.6
36.0	37.2
35.5	36.6
35.0	36.5
34.5	36.1
34.0	35.8
33.5	35.5
33.0	35.2
32.5	34.8
32.0	34.6
31.5	34.2
31.0	34.0
30.5	33.6
30.0	33.4
29.5	33.0
29.0	32.8
28.5	32.6
28.0	32.2
27.5	31.8
27.0	31.5

NEEDLE PROBE #3 -- DIGITAL THERMOMETER #1

Temperature - Chemical Thermometer	Temperature - Digital Thermometer
39.5	43
39.0	42.7
38.5	42.6
38.0	42.5
37.5	42.1
37.0	41.9
36.5	41.6
36.0	41.4
35.5	41.1
35.0	40.5
34.5	39.8
34.0	39.1
33.5	38.9
33.0	38.6
32.5	38.4
32.0	38.0
31.5	37.6
31.0	37.1
30.5	36.8
30.0	36.2
29.5	35.9
29.0	35.3
28.5	34.9
28.0	34.3
27.5	33.8
27.0	33.2

NEEDLE PROBE #1 ---- SCANNING THERMOMETER

Temperature - Chemical Thermometer	Temperature Scanning Tele Thermometer
50.0	49.1
49.5	49.0
49.0	48.5
48.5	48
48.0	47.0
47.5	47.5
47.0	46.2
46.5	46.0
46.0	45.5
45.5	45.2
45.0	45.0
44.5	44.9
44	44
43.5	44.0
43.0	43.5
42.5	43.0
42.0	42.5
41.5	42.3
41.0	42.0
40.5	41.9
40.0	41.5
39.5	40.9
39.0	40.7
38.5	40.3
38.0	39.9
37.5	39.5
37.0	39.2
36.5	38.9
36.0	38.7
35.5	38.1
35.0	37.9
34.5	37.3
34.0	36.9
33.5	36.5
33.0	35.8
32.5	35
32.0	34.9
31.5	34.5
31.0	34.3
30.5	34.0
30.0	33.8
29.5	33.1
29.0	33.0
28.5	32.8
28.0	32.5
27.5	32.0
27.0	29.7

NEEDLE PROBE #3 ----- SCANNING THERMOMETER

Temperature - Chemical Thermometer	Temperature Scanning Tele Thermometer above scale
50.0	
49.5	"
49.0	"
48.5	"
48.0	"
47.5	"
47	50
46.5	49.2
46.0	49.8
48.5	45.2
45.0	48.0
44.5	47.8
44.0	47.2
43.5	47.0
43.0	46.5
42.5	46.3
42.0	46.0
41.5	45.5
41.0	45.1
40.5	44.9
40.0	44.6
39.5	43.8
39.0	43.1
38.5	42.4
38.0	42.0
37.5	41.3
37.0	40.9
36.5	40.4
36.0	40.2
35.5	40.1
35.0	39.9
34.5	39.0
34.0	38.8
33.5	38.4
33.0	38.1
32.5	37.5
32.0	37.2
31.5	36.7
31.0	36.3
30.5	36.1
3.00	35.7
29.5	35.2
29.0	35.0
28.5	34.9
28.0	34.6
27.5	34.1
27.0	39.9

J. APPENDIX C - RELIABILITY TESTS AND PROCEDURES

1. Test of percent error of skinfold thickness measurement of triceps and forearm

The reliability of the experimenter in accurately measuring the skinfold thickness of the triceps and the forearm was tested in the following manner. The subject was repeatedly tested ten times for triceps and forearm skinfold thickness. A percent error test was then done for both the triceps and the forearm measurements. The procedure was as follows on each measurement. The subject was standing with the arm to be tested hanging relaxed by his/her side. For the measurement of the triceps skinfold thickness, a level halfway between the lateral tip of the acromion process and the proximal tip of the olecranon was marked. A pinch grasp of the subcutaneous tissue was taken at about one centimeter above the mark. The crest of the skinfold was parallel to the long axis of the arm. The caliper jaws were applied to the exact site where the skin was marked. The spring handles were released fully and when the pointer on the dial had steadied, a readoff of the measurement in tenths of millimeters was taken.

For the measurement of the forearm skinfold thickness, the subjects abducted their arm slightly so as to facilitate measurement. A level six centimeters distal to the medial epicondyle was marked on the medial border of the forearm. A pinch grasp of the subcutaneous tissue was taken about one centimeter above the mark. The crest of the skinfold was parallel to the forearm. The caliper jaws were applied to the exact site where the skin was marked. The spring handles were released fully and when the pointer on the dial had steadied, a readoff of the measurement in tenths of millimeters was taken. A percent error was then calculated on the ten repeated measurements of both the triceps and the forearm skinfold thickness.

2. Test of Percent Error of Calculation of Motor Nerve Conduction Velocity

The reliability of the experimenter in accurately calculating the motor nerve conduction velocity was tested in the following manner. Two sites of stimulation were marked on the forearm of a subject. Ten recordings of supramaximal stimulation of each site was recorded on TECA photographic paper. These 20 recordings were then coded and shuffled. All the horizontal lines (parallel to the base line of the action potential) and the vertical lines (drawn from the point of upward deflection perpendicular to the horizontal line) were drawn on the photographic paper first. Once this procedure had been completed on all the 20 recordings, the motor nerve conduction velocity was then

calculated for each recording. A test of percent error was then done on the repeated measurements of the 20 recordings of motor nerve conduction velocity. A code was made by the experimenter so as to match the identical recordings. Each of the recordings was calculated on two separate traits and then a reliability test was done. Furthermore, the identical recordings were then matched and another reliability test was done on these recordings.

3. Control of Experimenter's Bias in Calculation of Motor Nerve Conduction Velocity

In order to control for experimenter's bias in measurement of the motor nerve conduction velocity, the following procedure was used. The one minute pre-treatment, zero minute pre-treatment, zero minute post-treatment, one minute post-treatment recordings of motor nerve conduction velocity were coded, cut out and attached randomly onto a separate page. The experimenter was then able to calculate the motor nerve conduction velocity without knowing if that particular recording was a pre- or post-treatment recording.

4. Needle Probe Insertion

The competency of the experimenter in inserting a needle probe accurately and safely was evaluated by Dr. Anne Bellamy. See attached letter.



June 24, 1983.

TO WHOM IT MAY CONCERN:

Re: Yvette CLAVEAU

This letter is to certify that in my opinion Yvette Claveau has obtained the necessary expertise required to insert the subcutaneous needle for measuring temperature as required by her current research proposal. I have observed her technique in this needle insertion and I have no hesitation whatsoever in recommending that she be allowed to carry this out as part of her research study. If you require further information do not hesitate to contact me.

Sincerely,

L.A. Bellamy, M.D., FRCP (C)

/paa

University of
Alberta Hospital

Walter C. Mackenzie
Health Sciences
Centre

Aberhart Centre

Mewburn Veterans
Centre

University Hospitals
Hostel

University Hospitals
Industrial Services
Centre

K. APPENDIX D - RAW DATA COLLECTION FORMS

NAME:

DATE:

TIME:

ROOM TEMPERATURE:

TREATMENT:

SWD

US

HP

PROBE USED:

TRICEPS SKINFOLD THICKNESS:

FOREARM SKINFOLD THICKNESS:

SENSATION TEST HOT vs. COLD

DATA COLLECTION

	TEMPERATURE		MOTOR NERVE
	Probe	Converted	CONDUCTION VELOCITY
1 minute pre-treatment			
0 minutes pre-treatment			
During treatment:			
1 minute			
2 minutes			
3 minutes			
4 minutes			
5 minutes			
6 minutes			
7 minutes			
8 minutes			
9 minutes			
10 minutes			
11 minutes			
12 minutes			
13 minutes			
14 minutes			
15 minutes			
16 minutes			
17 minutes			
18 minutes			
19 minutes			
20 minutes			
0 minutes post-treatment post-treatment			
1 minute post-treatment			